

INSTALLATION MANUAL

A V A N T

REM*sp*TM



MedRx[®]

Contents

Getting to Know Your AVANT™ REMsp	3
Software Installation	4
Driver Installation- Windows 7	7
Driver Installation- Windows XP	10
EMC Precautions	11
Safety	14
Limited Warranty	16



#0086



www.medrx-usa.com



1200 Starkey Rd., #105, Largo FL 33771 U.S.A.

Toll Free: (888) 392-1234 • (727) 584-9600

Fax: (727) 584-9602 • Email: medrx@medrx-usa.com



MedRx's Authorized Representative in Europe

(Regulatory affairs only)

Emergo Europe, Molenstraat 15

2513 BH The Hague, The Netherlands

Getting to Know Your AVANT REMsp

Intended Use Statement:

The Avant series of REM (Real Ear Measurement) devices measure sound levels directly in patient's ears. They are used in the measurement and fitting of hearing aids for adults and children. These measurements can be done with or without the hearing instrument being worn. They are also used for hearing loss simulation. The REM can perform Live Speech Mapping, and MedRx's in-situ method for getting the fitting right the first time, every time. These devices should be operated by trained professionals with education and/or training in the field of audiometry.

Indication For Use Statement:

The Avant REM (Real Ear Measurement) devices are for use by professionals with education and/or training in the field of audiometry to evaluate the fitting of hearing aids and are used for hearing loss simulation in adults and children.

The AVANT REMsp represents a new era of precision in-situ verification for your office. Compact yet rugged, this PC-Based system is USB powered and supports ANSI and IEC Real Ear tests. The software includes targets for **DSL i/o 5.0** and **NAL-NL2**. The REMsp is an affordable, single probe device which utilizes MedRx's in-situ method for getting the fitting right the *first* time, *every* time. The following section of this manual will familiarize you with the physical features and accessories of the REMsp system. The Avant REMsp is a device that is used in measuring the real-ear acoustical characteristics of hearing aids. The device performs measurements of real-ear acoustical characteristics of a hearing aid on a given human ear, and does comply with the International Standards ANSI S-3.46 and IEC 61669.



Front View





Rear View

Use the accessories provided with your Avant REMsp. Use of un-approved accessories is not recommended.

Software Installation

Do Not Plug in the AVANT REMsp yet!

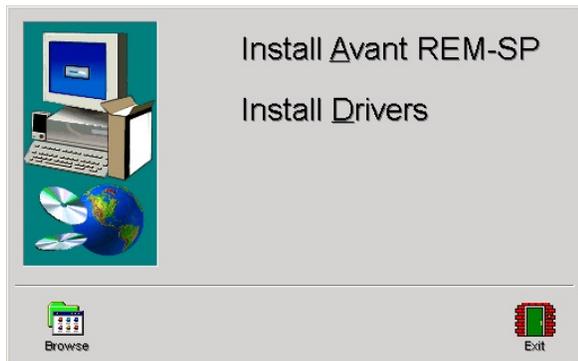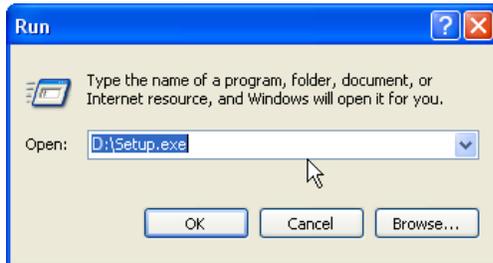

1. Insert the AVANT REMsp™ CD-ROM into the CD drive. Wait until the **Setup program starts**.

- If the Setup program does not automatically start:
- Press the “Win – R” keys on the keyboard.
- Type **D:\Setup.exe** in the window where ‘D’ is the drive letter assigned to the CD ROM drive on your computer.
- Press **OK** to start the Setup.


2. On the Setup screen, choose **Install Avant REM-SP**.

3. Wait for the program to setup the InstallShield Wizard.




4. This is the Welcome screen

- Click **Next**.

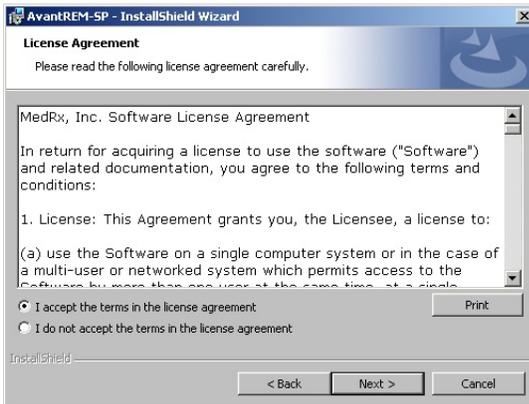

5. Read the Software License Agreement. This important document defines the acceptable usage of the REMsp software.

- After reading the Agreement, click **I accept**.
- Click **Next**.

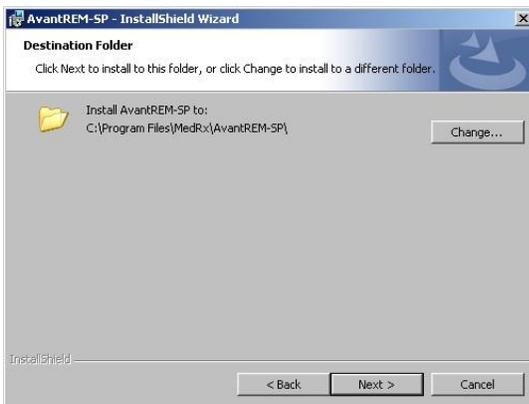

6. This screen indicates the location of the program files.


- Click **Next**.

Note: You can install the Software to a different location, but it is not recommended.



7. Choose desired language and locale

- Click **Next**.

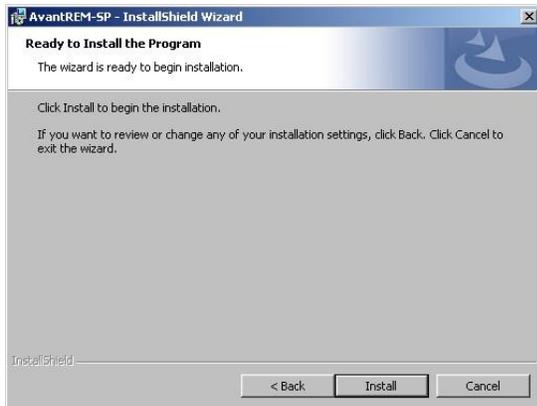

8. Ready to Install Program.

- Click **Install**.



9. Wait while the InstallShield Wizard installs the Avant REMsp program.

- Click **Next**.



10. When the installation is complete, click **Finish**.



Driver Installation - Windows 7


(see page 10 for Windows XP Driver Installation)

IMPORTANT – PLEASE READ BEFORE PLUGGING USB CABLE INTO YOUR COMPUTER



Your AVANT REMsp is powered by a USB cable connection to your computer.

1. Connect the AVANT REMsp™ to your computer as shown above, or use the included USB extension cable between the REMsp and the computer.
2. Wait for the system to copy and install default drivers. During this process, you will see the following message. “New Hardware has been found”.

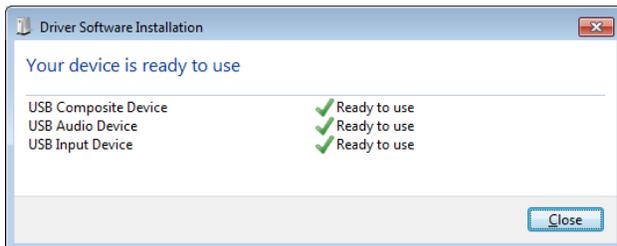


3. When this screen appears or a message in the bottom right corner appears “New Hardware is ready to use”, click **Close**.



4. On the Avant REM-SP Setup screen, click **Install Drivers**.




5. When this screen appears, click **Ok**.

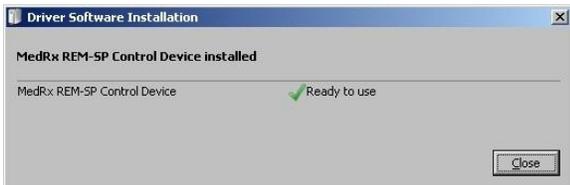


6. If this window appears and all devices are "Ready to use", click **Close**.

- Drivers installed successfully

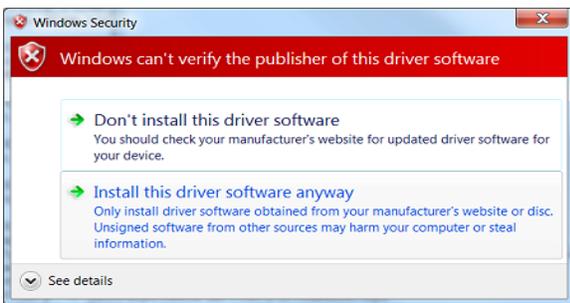


7. If this warning screen appears, click **Install this driver software anyway**.

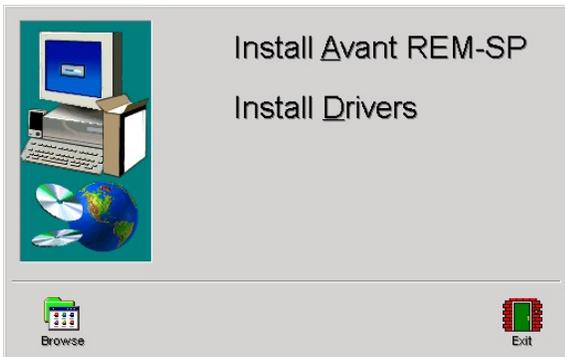


8. On Setup Window click **Exit**.

Next you need to confirm or set the Default Windows sound card settings. This will route all non-AVANT™ Windows sounds to the internal sound card of your computer. These sounds include event notifications such as new e-mail and error warnings as well as audio and video playback.




1. Launch the **AVANT REMsp** software.
2. Open the **Advanced Options** from File menu as shown.

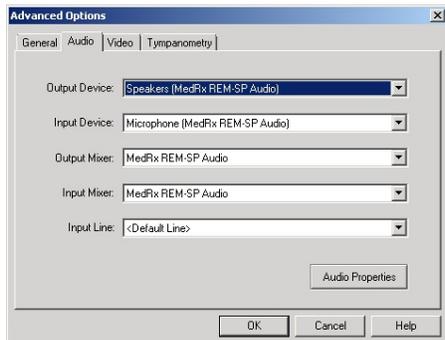

3. Open **Audio tab**.
4. When the audio properties are configured properly, during driver installation, the Audio Tab will appear like the image on the left. If not, use the pull-down lists to adjust the settings to match the image.


5. Click **Audio Properties**.

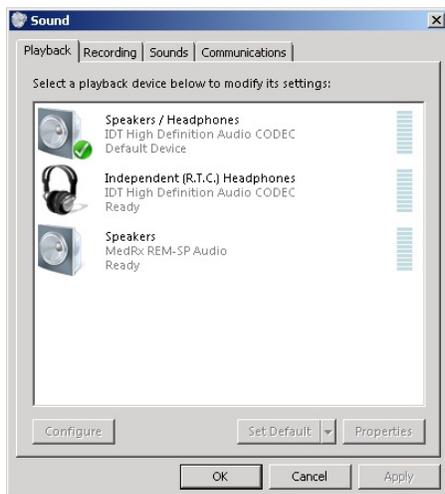

6. In Windows Sound control panel, make sure the MedRx Audio Device is not set as default. If it is default, change this by clicking on your system (non-MedRx) audio device and then choose Set Default.

NOTE: The internal sound card on your computer will likely not have the same name as this screen shot. Consult your computer's documentation for the name of the internal sound card and set this control accordingly.

7. On Setup Window click **Exit**

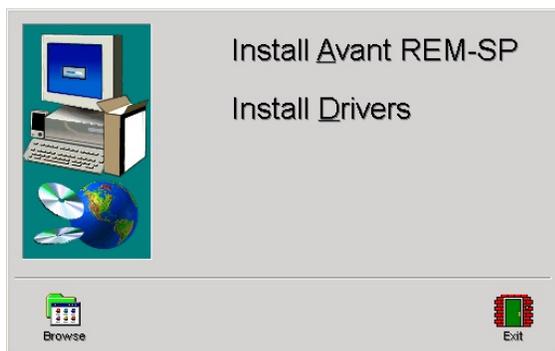

Driver Installation – Windows XP

IMPORTANT – PLEASE READ BEFORE PLUGGING USB CABLE INTO YOUR COMPUTER



Your AVANT REMsp is powered by a USB cable connection to your computer.

1. Connect the AVANT REMsp™ to your computer as shown above, or use the included USB extension cable between the REMsp and the computer.
2. Wait for the system to copy and install default drivers. During this process, you will see the following message. “New Hardware has been found”.



3. After the software has been installed and hardware has been recognized, and installed
 - Click **Install Drivers**.



4. When this screen appears,
 - Click **OK**



5. When this screen appears,
 - Click **Install**.



6. When the driver signature check screen appears,
 - Click '**Continue Anyway**'.
7. Continue the installation by following the default options when prompted.
8. Press **Exit** when finished.

Note: In Windows[®] XP, the drivers have to be loaded for every USB port the device is plugged in to.

EMC Precautions

The Avant REMsp needs special precautions regarding EMC and needs to be installed and put into service according to the following EMC information.

List of all cables and maximum lengths of cables, transducers and accessories:

Transducer / Accessories	Maximum Cable length
USB Cable	2,9 meters
All Speakers	2,9 meters



Warnings!

- The use of accessories and cables other than those specified, with the exception of transducers and cables sold by the manufacturer of the Avant REMsp as replacement parts for internal components, may result in increased emissions or decreased immunity of the Avant REMsp.
- The Avant REMsp should not be used adjacent to or stacked with other equipment and if adjacent or stacked use is necessary, the Avant REMsp should be observed to verify normal operation in the configuration in which it will be used.

- The Avant REMsp may be interfered with by other equipment, even if that other equipment complies with CISPR emission requirements.
- The Avant REMsp does not have life supporting function
- Portable and mobile RF communications equipment can affect the Avant REMsp.

Guidance and manufacturer's declaration – electromagnetic emissions		
The Avant REMsp is intended for use in electromagnetic environment specific below. The customer or the user of the Avant REMsp should assure that it is used in such an environment.		
Emission test	Compliance	Electromagnetic environment - guidance
RF emissions CISPR 11	Group 1	The Avant REMsp uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class B	The Avant REMsp is suitable for use in all establishments, including domestic establishments and those directly connected to the public low - voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions IEC 61000-3-2	Non applicable	
Voltage fluctuations / flicker emissions IEC 61000-3-3	Non applicable	

Guidance and manufacturer's declaration – electromagnetic immunity			
The Avant REMsp is intended for use in electromagnetic environment specific below. The customer or the user of the Avant REMsp should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
Electrostatic discharge (ESD) IEC 61000-4-2	+/- 6 kV contact +/- 8 kV air	+/- 6 kV contact +/- 8 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient / burst IEC 61000-4-4	+/- 2 kV for power supply lines +/- 1 kV for input / output lines	+/- 2 kV for power supply lines +/- 1 kV for input / output lines	Mains power quality should be that of a typical commercial or hospital environment.
Power frequency (50/60 Hz) Magnetic field IEC 61000-4-8	3 A/m	3 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

Guidance and manufacturer's declaration – electromagnetic immunity			
The Avant REMsp is intended for use in electromagnetic environment specific below. The customer or the user of the Avant REMsp should assure that it is used in such an environment.			
Immunity test	IEC 60601- test level	Compliance level	Electromagnetic environment - guidance
			Portable and mobile RF communications equipment should be used no closer to any part of the Avant REMsp, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter. Recommended separation distance:
Conducted RF IEC 61000-4-6	3 V _{eff}	3 V _{eff}	$d = 1,17 \times \sqrt{P}$
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 2,5 GHz	3 V/m	$d = 1,17 \times \sqrt{P}$ 80 to 800 MHz

			$d = 2,33 \times \sqrt{P}$ 800 MHz to 2,5 GHz
			<p>Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m).</p> <p>Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey ^a, should be less than the compliance level in each frequency range ^b.</p> <p>Interference may occur in the vicinity of equipment marked with the following symbol:</p> 
<p>NOTE 1 At 80 MHz and 800 MHz, the higher frequency ranges applies.</p> <p>NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.</p>			
<p>a Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the Avant REMsp is used exceeds the applicable RF compliance level above, the Avant REMsp should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the Avant REMsp</p> <p>b Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.</p>			

Recommended separation distances between Portable and mobile RF communications equipment and the Avant REMsp			
<p>The Avant REMsp is intended to use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the Avant REMsp can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the Avant REMsp as recommended below, according to the maximum output power of the communications equipment.</p>			
Rated maximum output power of transmitter W	Separation distance according to frequency of transmitter meters		
	150 kHz to 80 MHz $d = 1,17 \times \sqrt{P}$	80 MHz to 800 MHz $d = 1,17 \times \sqrt{P}$	800 MHz to 2,5 GHz $d = 2,33 \times \sqrt{P}$
0,01	0,12	0,12	0,233
0,1	0,37	0,37	0,74
1	1,17	1,17	2,33
10	3,7	3,7	7,40
100	11,7	11,7	23,3
<p>For transmitters rated at a maximum output power not listed above, the recommended separation distance d in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.</p> <p>NOTE 1 At 80 MHz and 800 MHz the separation distance for the higher frequency range applies.</p> <p>NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.</p>			

Safety

- Regarding electrical safety, this device is designed to be used only by professionals in the hearing healthcare industry.

- It is Class II Medical Electrical (ME) equipment that is part of an ME system.  This device provides

 Type B protection (Type B equipment, Type B applied part)

- This device is not protected from ingress of water. The water protection level is **IP20**.
- Power is supplied by the USB cable connected to a computer. The USB computer power must be able to supply at least 400mA at the standard USB voltage.
- A USB Optical Isolator, with a minimum of 1000 DC volt isolation, should be placed in-line between the computer's USB connection and the MedRx device. The Optical Isolator should be powered by a power supply that conforms to IEC 60601-1. The computer, Optical Isolator's power supply and the speaker's power supply should be connected to the Medical Grade isolation transformer that conforms to IEC 60601-1.
- The computer used with this device should conform to the requirements of IEC 60950-1 and IEC 60601-1-4.
- A MULTIPLE PORTABLE SOCKET-OUTLET or extension cord shall not be connected to the system.
- The device warm-up time is less than 2 minutes.
- Do not connect items that are not specified as part of the system.

- The use environment should be between 10°C and 35°C , humidity within 30% to 90%  and an atmospheric pressure range from 80 kPa to 104 kPa.
- Storage temperature range at least from 0°C to 50°C.
- All components with patient contact are made of bio-compatible materials.
- This device does not produce any adverse physiological effects.
- Install the device as directed by this manual to achieve optimal use. Clean accessories per the cleaning instructions prior to use. No Sterilization is required for components of this device. However, new probe tubes are needed for each patient where applicable and cleaning of the device and accessories should follow the procedure outlined below.
- The device is not intended to be operated in an environment with anesthetics, oxygen or NO. It is not an AP or APG device. **This ME System is not intended for use with flammable anesthetics.**
- This device uses Type B application parts temporarily placed on the patient during testing. They are nonconductive and can be immediately withdrawn from the patient at any time.
- The device is intended for continuous operation.
- The computer and the MedRx device or accessories may be located in the patient environment if required.
- The colored light on the device only signifies that the device is operational and the software is running (green). The colors do not signify any dangerous or faulty condition.

- Contact the local MedRx distributor for safe and proper disposal of this equipment.  Proper disposal may require that it be sent to collection facilities for recovery and recycling.
- All repairs should be sent to MedRx for evaluation and / or repair. However, necessary diagrams and repair instruction will upon request be provided to authorized repair personnel.
- There are no known contraindications for use of this equipment.

Symbols that may be used:



Read the instruction manuals for safe usage of the device. (operating instructions)



or SN Indicates that the device serial number will follow.



Type B applied part. (Type B equipment)



Manufacturer (MedRx)



Authorized Representative in Europe



Non-ionizing electromagnetic radiation



Special Disposal Required.



Humidity Limitation



Caution, General warning sign



Temperature limitation



Read the instruction manuals for safe usage of the device (operating instructions).



Class II equipment



Start (of action)



Stop (of action)



Percentile Setup



Calibration



Loudspeaker (Speaker)



Headphones



Microphone



Recording

Recommended Procedures for Cleaning and Disinfection

1. Probe Tubes are single use components, and should not be re-used by another patient.
2. It is recommended that 70% Isopropyl Alcohol should be applied to a soft clean cloth or tissue, not directly on the component to be cleaned. The cloth should never be wet, just damp. A mild soapy water solution is an alternative cleaning liquid.
3. To ensure that cross contamination does not occur, use clean cloth or sealed Alcohol swabs for each device to be cleaned.
4. Wipe the surfaces of the probe microphone, black ear loop and headphone pads with the 70% Isopropyl Alcohol. Clean other transducers in the same way. **Do not let 70% Isopropyl Alcohol or water enter the microphone sound inlet.**
5. The probe microphone cords and white device housing may also be wiped with 70% Isopropyl Alcohol. The speaker controls, headphone ear pads, head band and other components may be cleaned in a similar way.
6. Let all components that have been cleaned, thoroughly dry before use.
7. Cleaning of the computer should be performed using the methods suggested in the computer's manual.

Congratulations

Your MedRx system is now set up and ready for use. Please consult the Training Manual and the Interactive Help Files within the software for instructions and procedures. The Training Manual is available in PDF format on CD and at www.medrx-usa.com in our Download Section.

Limited Warranty

MedRx, Inc warrants this product to be free from defects in material and workmanship for one year from the time of purchase. If this system fails to perform as specified during this period, the purchaser is responsible for calling MedRx at (888) 392-1234 or (727) 584-9600. The company's representative will advise the owner to either return specific components or the entire system to:

**MedRx, Inc.
1200 Starkey Road #105
Largo, FL 33771 USA**

MedRx will repair or replace any defective devices, fully test the system and/or components and ship the system promptly back to the owner. There is no cost for the repair or return shipping, provided the system is one year old or less and has not been misused, abused or damaged. Such damage includes, but is not limited to, dropping, exposure to excessive heat greater than 100°F and water/liquid damage.

Repair or replacement of the system as provided under this warranty is the sole and exclusive remedy of the purchaser. MedRx shall not be liable for any consequential or incidental damages or for breach of any express or implied warranty. Except to the extent of applicable law, any implied warranty, merchantability or fitness of this product is limited to the duration of this warranty.

MedRx will, at its discretion, service and repair out of warranty products at the purchaser's request, charging for parts and labor as necessary.

The limited warranty is deemed void if software or hardware is installed on this product which is not pre-approved by MedRx, Inc. Approved software includes NOAH™ and HIMS A approved hearing aid manufacturer programming modules for fitting hearing aids.

MedRx, Inc is not responsible for problems resulting from installation of unapproved software or hardware. In the event of unapproved software or hardware installed on the system causing a conflict, MedRx will service the product for a fee to be determined at the time of service.

Any extension of this warranty past the initial one-year warranty is subject to the following (where applicable).

1. A \$300 deductible per repair.
2. Extended warranty does not include cables, connectors or peripherals.
3. Extended warranty of the Video Otoscope covers optics only.