



MedRx[®]

Otowave 102 Operating Manual
Applies from serial number 37400 onwards





0123

TÜV SÜD Product Services GmbH
Ridlerstraße 65 • 80339 Munich • Germany



Amplivox Ltd
3800 Parkside, Solihull Parkway,
Birmingham Business Park, Birmingham,
West Midlands,
B37 7YG

www.amplivox.com



MedRx's Authorized Representative in Europe
DGS Diagnostics A/S
Audiometer Alle 1 • 5500 Middelfart • Denmark

Distributors:



1200 Starkey Rd., #105, Largo, FL 33771 U.S.A.
Toll Free: (888) 392-1234 • (727) 584-9600
Fax: (727) 584-9602 • Email: medrx@medrx-diagnostics.com
www.medrx-diagnostics.com

MedRx International
c/o MAICO Diagnostics GmbH
Sickingenstr. 70-71, 10553 Berlin, Germany
Tel.: +49 30/70 71 46-50
Fax: +49 30/70 71 46-99
Email: medrx-sales@maico.biz
www.medrx-diagnostics.com

TABLE OF CONTENT

1. INTRODUCTION	4
1.1. THANK YOU	4
1.2. INTENDED APPLICATIONS	4
1.3. FEATURES	4
1.4. UNPACKING	4
1.5. STANDARD CONTENTS AND OPTIONAL ACCESSORIES	5
1.6. GUARANTEE	5
1.7. WARNINGS	5
2. IMPORTANT SAFETY INSTRUCTIONS	6
2.1. PRECAUTIONS	6
2.2. ELECTROMAGNETIC COMPATIBILITY (EMC) CONSIDERATIONS	6
3. PRINCIPLES OF OPERATION	7
3.1. COMPLIANCE MEASUREMENT	7
3.2. TYMPANOGRAM	7
3.3. STAPEDIAL REFLEX MEASUREMENT	7
4. USING THE OTOWAVE	8
4.1. INSTALLING & REPLACING BATTERIES	8
4.2. OPERATING LANGUAGE	8
4.3. CONTROLS AND INDICATORS	9
4.4. THE PROBE	10
4.5. START-UP AND MENU DISPLAYS	10
4.6. INITIAL SETTINGS	11
5. TAKING MEASUREMENTS	12
5.1. PRIOR TO TESTING AND AMBIENT CONDITIONS	12
5.2. EAR TIP(S)	12
5.3. PERFORMING A TEST	12
5.4. EAR SEAL CHECK	16
5.5. ERROR MESSAGES	17
6. CONFIGURATION	17
6.1. SWEEP SETTINGS	17
6.2. REFLEX OPTIONS	18
6.3. SYSTEM SETTINGS	19
7. SAVING RESULTS IN THE INTERNAL DATABASE	20
7.1. GENERAL	20
7.2. DATA ENTRY	20
7.3. DATABASE FULL	21
8. IRDA COMMUNICATIONS	22
9. TRANSFERRING THE RESULTS	23
9.1. SENDING THE RESULTS TO A PRINTER	23
9.2. DATA TRANSFER TO NOAH OR MEDRX STUDIO	23
10. DATA MANAGEMENT	24

10.1.	LIST RECORDS	25
10.2.	DELETE RECORDS	25
10.3.	PRINT RECORDS	25
10.4.	SEND RECORDS TO A COMPUTER	25
11.	PERFORMING DAILY CHECKS	26
12.	SYSTEM INFORMATION	27
13.	ROUTINE MAINTENANCE	28
13.1.	CLEANING THE OTOWAVE	28
13.2.	EAR TIP AND PROBE	28
13.3.	CALIBRATION AND REPAIR OF THE INSTRUMENT	28
14.	ERROR MESSAGES & FAULT CONDITIONS	29
15.	TECHNICAL SPECIFICATION	31
15.1.	PERFORMANCE	31
15.2.	EQUIPMENT CLASSIFICATION	33
15.3.	SYMBOLS	34
16.	ORDERING CONSUMABLES AND ACCESSORIES	35
17.	DISPOSAL INFORMATION	35
18.	EMC GUIDANCE & MANUFACTURER'S DECLARATION	36
19.	USE WITH NON-MEDICAL ELECTRICAL EQUIPMENT	40

1. INTRODUCTION

1.1. THANK YOU

Thank you for purchasing an MedRx Otowave 102, a hand-held, portable tympanometer that will give many years of reliable service if treated with care. This operating manual covers product variants 102-1 & 102-4.

1.2. INTENDED APPLICATIONS

The Otowave 102 is designed for use by audiologists, general practitioners, hearing aid dispensers and child health professionals.

The instrument performs two types of measurement:

Tympanometry is used to measure the compliance of the tympanic membrane and middle ear at a fixed frequency over a range of pressures.

Reflex tests are used to measure stapedial reflexes. The Otowave measures ipsilateral reflexes and, when selected, reflex measurement is automatically carried out after a tympanogram is taken.

1.3. FEATURES

- Automatic measurement of ear canal volume, tympanic compliance peak, placement of the peak and the gradient
- Automatic detection of stapedial reflexes
- Up to 32, dual-ear patient tests can be stored in non-volatile memory
- Configurable settings for user preferences, held in non-volatile memory
- Printout via an infrared (IrDA) link to one of two thermal printers that may be selected by the user
- Data transfer to a computer via an infrared IrDA link for storage viewing & printing using either the MedRx Studio software or the NOAH application
- English, French, Spanish, Portuguese, Italian or German operating languages (user-selectable)

1.4. UNPACKING

Please check the contents of the shipping carton against the delivery note to make sure that all items ordered have been included. If anything is missing, please contact the distributor who supplied your instrument or MedRx, Inc. if you purchased direct.

Please retain the original shipping carton and packaging to transport the tympanometer for annual calibration or repair.

1.5. STANDARD CONTENTS AND OPTIONAL ACCESSORIES

STANDARD COMPONENTS			
Otowave 102 Tympanometer	8507930	Set of disposable ear-tips	8029344
USB stick with Software (MedRx Studio and Noah impedance module) and Operating Manuals	8517685	4 in 1 cavity assembly (0.2 ml/0.5 ml/2.0 ml/5.0 ml)	8011362
4 x 1.5 V 'AA' Batteries	8011226	Carrying case	8004651
Calibration certificate	8011512		

OPTIONAL COMPONENTS			
Additional sets of ear tips	8029344	Probe tip	8002592 ¹
Portable thermal printer (Standard in US conf.)	8503007	Seal (in probe tip)	8002009 ¹
Additional rolls of thermal printer paper (Standard in US conf.)	8029305	Infra-red USB Adapter	8105188



1.6. GUARANTEE

All the manufacture instruments are guaranteed against faulty materials and manufacture. The instrument will be repaired free of charge for a period of three years from the date of dispatch if returned, postage paid to the MedRx, Inc. service department. Return postage is free of charge for customers in the US and chargeable for overseas customers.



WARNING

The following exceptions apply:

- The pressure pump and transducers may go out of calibration due to rough handling or impact (dropping)

The lifetime of probe, probe seals and ear tips is dependent upon conditions of use. These parts are only guaranteed against faulty materials or manufacture.

1.7. WARNINGS

Throughout this manual, the following meanings of warnings and cautions apply:



WARNING

The WARNING label identifies conditions or practices that may present danger to the patient and/or user.



CAUTION

The CAUTION label identifies conditions or practices that could result in damage to the equipment.

¹ Applied part as according to IEC 60601-1

2. IMPORTANT SAFETY INSTRUCTIONS



WARNING

The Otowave 102 instrument must be used only by practitioners qualified to perform tympanometric tests. It is intended for transient use as a screening and diagnostic tool; however, no surgical or medical procedure should be undertaken solely on the basis of results obtained from the instrument.

2.1. PRECAUTIONS

READ THIS OPERATING MANUAL BEFORE ATTEMPTING TO USE THE INSTRUMENT

The tympanometer is for indoor use only and should be used only as described in this manual.

Refer to the precautions specified in Section 4.1 regarding the use of batteries.

Before the first use of the instrument each day, or if suspect or inconsistent results are apparent, the checks specified in Section 11 must be carried out. If these do not give the results specified, the instrument must not be used.

Never insert the probe into a patient's ear canal without a suitable ear tip fitted to the probe.

Use only the recommended disposable ear tips. These are for single use only - that is, each ear tip is intended to be used once only for a single ear for a single patient. Do not reuse ear tips as this will pose the risk of ear-to-ear or patient-to-patient cross-infection.

Do not immerse the unit in any fluids. See Section 13 of this manual for the proper cleaning procedure for the instrument and its accessories and the function of single-use parts.

Do not use the instrument in an oxygen-rich environment or in the presence of a flammable anaesthetic mixture or other flammable agents.

Do not drop or otherwise impact this instrument. If the instrument is dropped or damaged, return it to the manufacturer for repair and/or calibration. Do not use the instrument if any damage is suspected.

The instrument must be stored and used indoors within the specified temperature, pressure, and humidity ranges, see Section 15.

As with all instruments of this nature the measurements taken will be influenced by significant changes in altitude & pressure. The Otowave 102 tympanometer must be re-calibrated (for volume measurement only) at the intended operating elevation if it is to be used at elevations greater than 1000m above mean sea level. This applies to volume measurements up to 2.0ml maximum. Please refer to the service manual for more information.

Do not attempt to open, modify, or service the instrument. Return the instrument to the manufacturer or distributor for all repair and servicing requirements. Opening the instrument will void the warranty.

2.2. ELECTROMAGNETIC COMPATIBILITY (EMC) CONSIDERATIONS

Medical electrical equipment needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information in Section 18. This provides guidance on the electromagnetic environment in which to operate the instrument.

Portable and mobile radiofrequency (RF) communications equipment can affect medical electrical equipment. The instrument should not be used adjacent to or stacked with other equipment; if this is unavoidable the instrument should be observed to verify normal operation.

3. PRINCIPLES OF OPERATION

Please note: This operating manual is not intended as a training manual for tympanometry. The reader should consult standard audiology texts for the theory and application of the screening tests provided by this instrument.

3.1. COMPLIANCE MEASUREMENT

The Otowave 102 measures the compliance of the tympanic membrane and middle ear by playing a continuous 226Hz tone into the ear canal at a level calibrated to give 85dB SPL into a 2ml cavity. The sound level this produces in the ear canal is measured using a microphone and the compliance calculated from the result. In line with normal audiometric practice compliance is displayed as an equivalent volume of air in ml.

3.2. TYMPANOGRAM

To record the tympanogram the compliance is measured while the air pressure in the ear canal is varied from +200daPa to -400daPa by means of a small pump. The compliance peaks when the air pressure is the same on both sides of the tympanic membrane. The changing compliance with pressure is displayed as a graph.

3.3. STAPEDIAL REFLEX MEASUREMENT

Using the same principal it is also possible to establish whether a stapedial reflex is present. In this case, the 226Hz tone is used to measure the compliance of the ear, while a short tone at a different frequency is presented (the reflex stimulus). The level of this stimulus is increased in steps until the stapedial muscles respond causing the tympanic membrane to become stiffer, or a pre-set maximum level is reached. When the change in compliance exceeds a predetermined threshold, this constitutes a reflex and the change in compliance at that level when the stimulus is applied is displayed as a plot against time.

The stapedial reflex is measured at the static ear canal pressure that produces the maximum membrane compliance, so reflex measurements are taken after the tympanogram is measured when the peak compliance pressure has been established.

The Otowave model 102-1 measures stapedial reflex at 1000Hz, while the model 102-4 measures at 500Hz, 1000Hz, 2000Hz and 4000Hz. The maximum level for the reflex stimulus may be pre-set, along with the step size in dB between the three preceding lower levels of stimulus.

4. USING THE OTOWAVE

4.1. INSTALLING & REPLACING BATTERIES

The Otowave 102 may be powered from Alkaline 'AA' batteries or rechargeable Nickel-Metal Hydride (NiMH) batteries. Four batteries are required. Do not mix battery types or old and new batteries.

If the Otowave is to be used infrequently the use of alkaline cells is recommended. NiMH batteries have a high self-discharge rate and are likely to need recharging if left unused for several weeks.

Remove batteries from the instrument if it is not going to be used for more than a year.

The type of cell fitted must be set in the CONFIGURATION menu. By default, this is ALKALINE. Change the setting in the CONFIGURATION menu (scroll to BATTERY TYPE as described in Section 6).

To fit the cells, remove the battery compartment cover on the base of the tympanometer. Fit the cells as indicated inside the battery compartment and replace the battery compartment cover.



WARNING

Batteries should only be changed outside the patient environment. The operator should not touch the battery connectors and the patient simultaneously.



Changing the batteries does not affect the configuration, the contents of the database, the calibration settings or the results of the last test.

Note that local regulations are likely to cover disposal of used batteries.

4.2. OPERATING LANGUAGE

To set the operating language (English, French, Spanish, Portuguese, Italian or German) use the options within the CONFIGURATION menu (see Section 6).

4.3. CONTROLS AND INDICATORS

Press the On/Off key momentarily to turn the Otowave on or off (refer to the diagram below).



No warm-up time is required, although a short diagnostic routine will run for a few seconds. During this time the internal pump will operate. To switch off, again press the On/Off key momentarily.


Press the up ▲ and down ▼ navigation keys to scroll through the menus or set values

Press the right navigation key ► to accept a menu choice or go to the next step.

Press the left navigation key ◀ to cancel an operation or go back to the previous step.

The function of the left and right keys is usually shown on the bottom line of the display.

When not performing a test the Otowave 102 will switch off automatically after 90 or 180 seconds if no key is pressed (see Section 6 to make this selection).

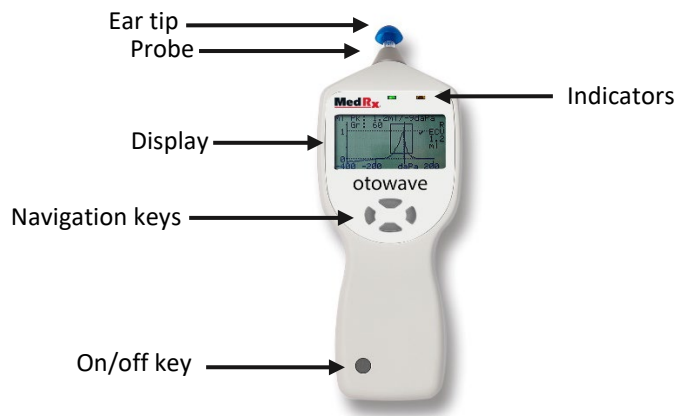


The indicators show the status of the system. Typical indications during a measurement sequence are as follows:

STATUS	LED A	LED B
Otowave turned off	Off	Off
Idle, test completed or test cancelled	On	Off
Insert probe or remove probe (refer to display for details)	Flashing (fast)	Flashing (fast)
Ensure probe is held steady while an ear seal is obtained	Off	Flashing (slow)
Testing - tympanogram and/or reflex measurement	Flashing (slow)	Off

For a full description of indicators used, messages displayed, and possible error conditions refer to Section 14.

4.4. THE PROBE

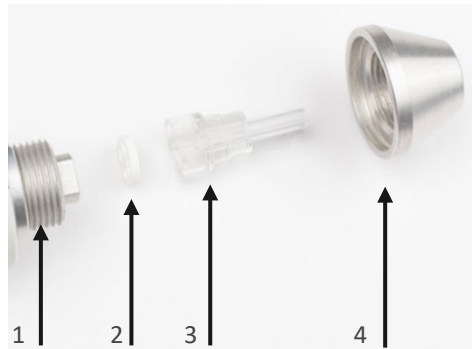

- | | | |
|----------|---------------------|--|
| 1 | Boss and Nut | Connection on probe body for attaching nose cone |
| 2 | Seal rubber | Gasket used to ensure air flow |
| 3 | Probe tip | Transparent probe tip housing the seal rubber |
| 4 | Nose cone | Top part of probe to securely fasten probe tip and seal rubber |

The small holes through the Otowave probe tip must be kept clear. If these become blocked a warning message will be displayed. The probe tip must be replaced.


To remove the probe tip, unscrew the nose cone and remove the probe tip from the boss. A small seal will be found in the base of the probe tip. This should be examined and replaced if it is blocked or damaged. Do not remove the nut securing the boss to the body of the instrument.



After replacing the tip, a Daily Check should be carried out (see Section 11).

4.5. START-UP AND MENU DISPLAYS

When the Otowave 102 is turned on the start-up screen is shown while internal tests are performed, and the pump is initialised. When the start-up sequence is complete the MAIN MENU is displayed:

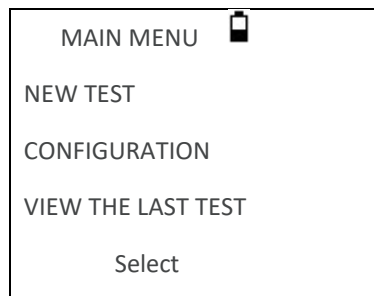

Use the navigation keys to scroll through and select menu options.

4.6. INITIAL SETTINGS

Use the CONFIGURATION options (see Section 6) to select the following options as required:

- display contrast for ease of viewing
- correct local date and time
- date format (DD/MM/YY or MM/DD/YY)
- correct battery type
- power-off delay (90 or 180 seconds)
- correct printer type (if used)

5. TAKING MEASUREMENTS

5.1. PRIOR TO TESTING AND AMBIENT CONDITIONS

A qualified health care professional should perform a thorough otoscopic examination to establish that the condition of the ear is suitable for the test options selected and that no contraindications are present. The latter would include obstruction of the external ear canal due to excessive wax and/or hairs, both of which would need to be removed.

Tympanometric and reflex testing should always be performed in a quiet room or in an acoustic booth.

5.2. EAR TIP(S)



Video available on how to choose the right ear tip.

These must be selected and fitted by a practitioner qualified to perform tympanometric tests.




Refer to Section 16 regarding these single-use parts.

5.3. PERFORMING A TEST




Having selected the required test settings a typical tympanogram measurement and reflex tests are carried out as follows.


From the MAIN MENU select NEW TEST:

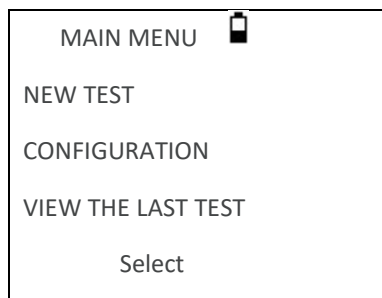



Select the ear(s) required for test:

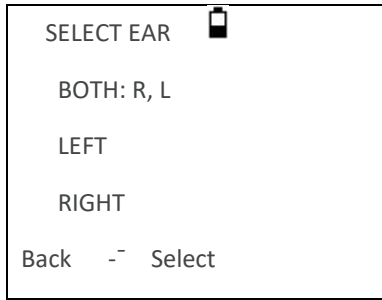


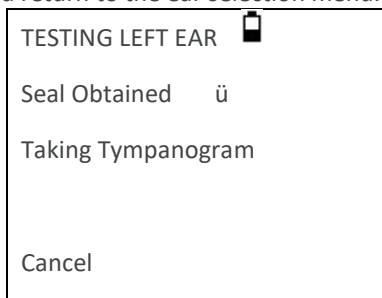
The message “Deleting last test” will be displayed momentarily followed by a message to insert the probe into the ear to be tested:

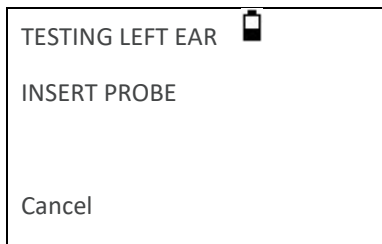

Present the ear tip to the ear and obtain a seal. If a good seal has been detected the following sequence of messages will be seen

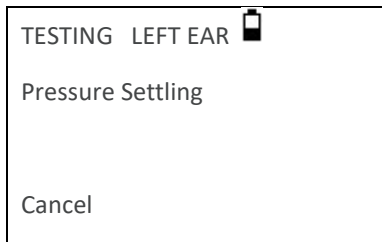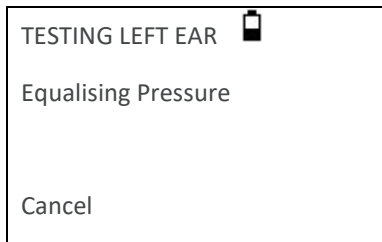


Press  at any time to cancel the test and return to the ear selection menu.



Once an adequate seal is detected the tympanogram measurement is made. This takes about 3 seconds. It is important not to move the probe and to ask the patient to remain very still during the test.

When the tympanogram is complete the instrument will perform the reflex test(s), if selected. By default, this test is only performed if a peak is found in the tympanogram. This and other reflex test options may be changed in the CONFIGURATION menu, see Section 6.


Before starting the reflex test the ear canal pressure will be set to the value that gave the peak compliance during the tympanogram test. The instrument will then step through the tone frequencies and levels set in the CONFIGURATION menu searching for a reflex response.

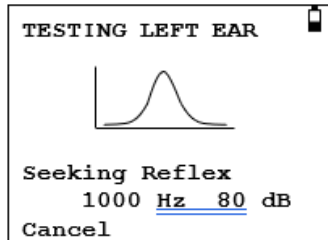

The display changes to show the frequency and level being used, starting with the lowest frequency and level selected.

When the measurement is complete the indicator on the instrument changes from flashing green to steady green. The display confirms that the test has been completed along with the instruction WITHDRAW PROBE.

Remove the ear tip from the patient and after a short period the tympanogram will be displayed.

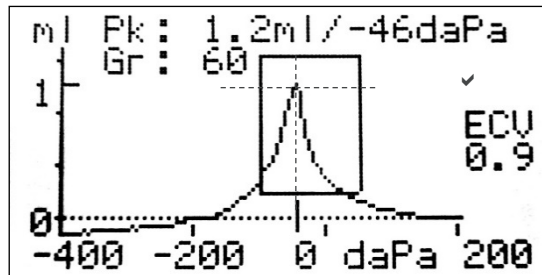

The display shows:


- The peak compliance, in ml (Pk)
- The pressure which gave the peak compliance in daPa
- The Gradient, in daPa (Gr)
- The Ear Canal Volume (ECV) in ml measured at 200 daPa.
- A pass/refer sign indicating if tympanogram appears to be normal or not
- A plot of compliance against pressure.
- Normative box (based on BSA recommendations)
- Pass (✓) / Refer (x) sign when tympanogram peak falls into normative box or not (refer)
- Pressure cursor to be operated with up ▲ and down ▼ navigation keys.

Review the tympanogram to ensure that the peak compliance point selected by the Otowave is suitable. If required, it is possible to select an alternative peak using the ▲ and ▼ keys. The figures displayed will change to reflect the peak selected and will be saved with the tympanogram.

To repeat the test, press ◀.

When satisfied with the tympanogram press ▶.

If reflex test(s) were carried out these results will now be displayed:

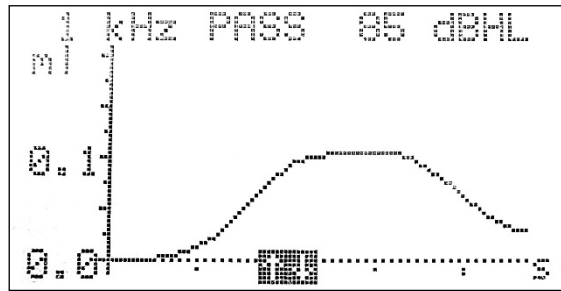

The display shows:

- The frequency and level of the reflex stimulus
- “PASS” if a reflex was found, else “x” (No Response)
- A plot of compliance against time

If the reflex test was performed at more than one frequency use the ▲ and ▼ keys to view the results for the other frequencies.


If the Otowave 102 was set to test for a reflex at all levels of the stimulus press ► to view an additional display following the reflex graphs. This shows a summary of the levels and frequencies at which a reflex was detected. The dash symbol “-” is shown if a reflex tone was not presented at the level indicated.

REFLEX SUMMARY				
dB				
100	ü	ü	x	-
90	ü	x	ü	ü
80	x	ü	ü	ü
70	x	ü	x	x
	Hz 500	1k	2k	4k

Press ◀ to return and view the tympanogram, reflex results or to repeat the test. When satisfied with the results press ►.

The message “Saving as last test” will be displayed and the results will be saved in the “last test” memory. The results will remain available until a new test is started, even if the Otowave is turned off.

If both ears were chosen for test the entire sequence will now be repeated for the right ear:

TESTING RIGHT EAR 
 INSERT PROBE
 Cancel Skip

Press ► to skip testing of the right ear and display the PROCESS RESULTS menu. Press ◀ to cancel and return to the ear selection menu. In both cases the left ear results are retained and may be viewed as the LAST TEST.

Otherwise insert the probe; the right ear test will then proceed as described above.

When the selected ears have been tested and the results saved the PROCESS RESULTS menu will be displayed. This accesses the following functions:

- Print the results
- Send the results to a computer
- Save the results in the internal database
- Review the results as described above
- Return to the main menu


The results of the last test performed remain available even if the Otowave has been turned off. To view these results select VIEW THE LAST TEST from the main menu. After selecting the required ear, the tympanogram will be displayed. It will then be possible to view the results and select the PROCESS RESULTS menu as if the test had just been completed.



5.4. EAR SEAL CHECK

The type of ear seal check employed at the start of a test can be set in the CONFIGURATION menu (Section 6). The default QUICK option is adequate for most tests, although it may not always be possible to generate the extremes of pressure with this setting.

However, if difficulty is experienced in using the ear tips to create a seal the alternative THOROUGH option may be helpful. This checks that a range of pressures will be available before starting a test by means of a visual indication of the quality of the seal:

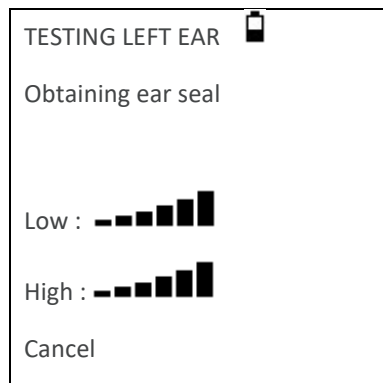

The number of bars shown indicates the robustness of the seal. The probe should be adjusted in the ear until two or more bars are shown for Low & High.

5.5. ERROR MESSAGES

The following error messages may be seen during the test sequence.

MESSAGE DISPLAYED	INDICATOR STATUS	LIKELY CAUSE(S)
WITHDRAW PROBE	Yellow Flashing	The probe has been moved during measurement. Re-insert the probe to repeat the test.
Volume outside range WITHDRAW PROBE	Yellow Flashing	The ear canal volume is above the 5ml. This message can also occur when the probe is not properly inserted into the ear.
Blocked ear WITHDRAW PROBE	Green Flashing	The ear canal volume is below 0.1ml. Check that the probe is not blocked and correctly inserted into the ear.
INSERT PROBE	Yellow Flashing	The seal was lost. Reinsert the probe to repeat the test.

6. CONFIGURATION

6.1. SWEEP SETTINGS




Video available on how to add ipsilateral reflexes to test protocol.

ITEM	DESCRIPTION	DEFAULT
Test Sequence:	When testing both ears, define what ear side the test will start with.	R, L
Ear Seal:	<p>The STANDARD option is adequate for most tests, although it may not always be possible to generate the extremes of pressure during a tympanogram measurement with this setting.</p> <p>If difficulty is experienced in using the ear tips to create a seal the alternative EXTENDED option may be helpful. This function checks that a range of pressures will be available before starting a test by means of a visual indication of the quality of the seal.</p> <p>The EXTENDED function is especially helpful if small ear canal volumes should not experience excessive pressure.</p>	Standard
Defaults:	Reset the sweep settings of the selected profile(s) to its original settings.	

6.2. REFLEX OPTIONS



Video available on how to add ipsilateral reflexes to test protocol.

ITEM	DESCRIPTION	DEFAULT
Level Mode:	 <p>ONE LEVEL: Use the S keys to choose the level of reflex stimulus to apply. Only one level will be tested in the measurement. The maximum level of ipsilateral stimulus may be set to maximum 100dBHL; the maximum level of contralateral stimulus may be set to 110dBHL.</p> <p>MULTILEVEL: Use the S keys to choose the maximum level of reflex stimulus to apply and the step size between the levels of the preceding stimuli. The maximum level of ipsilateral stimulus may be set between 85dBHL and 100dBHL; the maximum level of contralateral stimulus may be set between 85dBHL and 110dBHL.</p>	Multilevel
Levels:	Use the ▲ and ▼ keys to choose the maximum level of reflex stimulus to apply and the step size between the levels of the preceding stimuli. The maximum level of stimulus may be set between 85dBHL & 100dBHL. Press the ► key to confirm the selection or the ◀ key to cancel.	95 dB 5 dB steps
Frequencies:	Use the ▼ key to scroll through the frequencies available for each of the ipsilateral stimuli (1000Hz (102-1 option) or 500Hz, 1000Hz, 2000Hz & 4000Hz (102-4 option)), and then the ▲ key to select (ü) or deselect (-) the frequencies at which the reflex stimulus is to be applied. Then press ► to save the entire selection.	1kHz ipsi
Selection:	Use the ▲ and ▼ keys to choose the circumstances when a reflex measurement is to be made (always, never, only if a compliance peak is found, or only after confirmation is made at the start of the test sequence). In cases where a compliance peak has not been established a pressure of OdaPa is used. Press the ► key to confirm the selection or the ◀ key to cancel.	Only if peak found
Threshold:	Use the keys to choose the change in compliance required to signify that a reflex response has been detected (0.01ml to 0.5ml). The default is 0.03ml.	0.03 ml
Auto-Stop:	By default, the reflex test at each frequency will stop at the lowest level of stimulus that produces a response. By setting REFLEX AUTO-STOP to NO the Otowave 102 will test for a reflex at all selected levels. (Note that 100dBHL at 4000Hz is not available).	No

Polarity:	Define the polarity of the reflex graphs, if the reflex is plotted upwards (UP) or downwards (DOWN).	Up
Filter:	Use the keys to choose either 2Hz or 1.5Hz. The default of 2Hz is suitable for most circumstances. However, if a smoother reflex plot is required for better interpretation 1.5Hz may be chosen.	2 Hz
Defaults:	Reset the sweep settings of the selected profile(s) to its original settings.	

6.3. SYSTEM SETTINGS

ITEM	DESCRIPTION	DEFAULT
Time/Date:	Set the internal clock date and time. Use the ◀ and ▶ keys to select a field and the ▲ and ▼ keys to adjust the value.	
Printer	Select thermal printer you want to use with the unit (Sanibel MPT-II or Able AP1300).	MPT-II
Battery Type	Select what kind of batteries are used with the unit (primary or rechargeable).	Primary
Power-Off Delay	Adjust the time when device shuts off to save power.	90 s
Contrast:	Adjust the display contrast using the ▲ and ▼ keys.	
Cal. Dates:	Select PRINT CAL. DATES to show the serial number for the base unit and the transducers on the print-out provided by the Sanibel Thermal printer.	PRINT CAL. Dates
Date Mode:	Set the format of how the date is displayed: DD/MM/YY or MM/DD/YY	DD/MM/YY
Hospital:	Allows the Hospital name to be entered. The name will appear at the top of the printout.	
Department:	Allows the Department name to be entered. The name will appear at the top of the printout.	
Language:	Change the operation language to English, German, French, Spanish, Portuguese or Italian.	English
Defaults:	Reset the sweep settings of the selected profile(s) to its original settings.	

7. SAVING RESULTS IN THE INTERNAL DATABASE

7.1. GENERAL

Up to 32 tests can be saved in the Otowave 102 internal database.

To save the results of a test select SAVE RESULTS from the PROCESS RESULTS menu that is displayed on completion of a test. This option can also be accessed by selecting VIEW THE LAST TEST from the main menu and scrolling through the results using the ► key as long as the test results have not already been saved or deleted (e.g. by starting and then aborting a new test).

A three-character identifier is used for the record. This is also used as the reference for the patient's name on the printed record and for data transferred to a computer. The identifier would typically be the patient's initials, and as the tympanometer uses a combination of this identifier and the date/time of a test to refer to stored records this same identifier may be used for different tests for the same patient.

7.2. DATA ENTRY

PATIENT INITIALS 

ABCDEFGHIJKLM

NOPQRSTUVWXYZ

-01233456789

Hold to enter / cancel

To enter the identifier:

- Use the ▲, ▼, ◀ and ▶ keys to select a character.
- Press and hold the ▶ key to enter the selected character.
- Press and hold the ◀ key to delete the last character.

To save the test results:


- Enter all three characters for the identifier.
- Press and hold the ▶ key to save the record.

To cancel saving the last test:

- Delete any characters that have been entered.
- Press and hold the ◀ key.

7.3. DATABASE FULL

A warning will be displayed if the database is full when attempting to save a test:

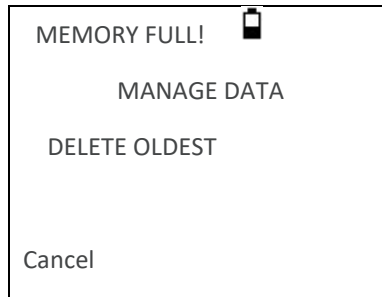

Selecting MANAGE DATA will display the DATA MANAGEMENT menu which provides options for printing or transferring data to a computer prior to deleting records to make space for the new test.

DELETE OLDEST will overwrite the oldest record in memory with the results being stored. Cancel will return to the previous menu.

8. IRDA COMMUNICATIONS

The Otowave 102 can send test results to a designated printer or a suitably equipped computer via an infra-red link.

If the computer does not have an infra-red port a suitable infra-red adapter will be required. The ACTYSIS ACT-IR2000U USB adapter is specified for and has been tested for use with the Otowave 102. This adapter may be purchased from MedRx and only this device should be used for this purpose.

The Otowave sends data through a small window on the right of the probe. For a printer the data is received through a window in the front of the printer; for a computer the data is received through a window located either on the case or on the plug-in adapter if this is used.

The environment in which the Otowave is used can affect the data transfer process. The following are recommendations but may need to be modified depending on the environment.

- The two communication windows should be in line and pointing directly at each other, 10-20cm apart
- Both units must be out of direct sunlight for optimum communication
- For transferring data to a printer ensure that no computer or printer other than the one to be used is within range
- Similarly, for transferring data to a computer ensure that no other IrDA device is within range
- The infra-red link must not be broken once a connection between the printer/computer and the Otowave has been established
- If the printer/computer or Otowave are moved, or an object between them breaks the link, the data may become corrupted or the Otowave may not respond to the controls until the data transfer process has timed out (this could take 30 to 40 seconds); this may also occur if the printer batteries are discharged while attempting to print

Once the data transfer process has timed-out the resulting error message can be cleared, and the data re-sent; if the data is still corrupted select Cancel on the Otowave and then send the data again.

9. TRANSFERRING THE RESULTS

9.1. SENDING THE RESULTS TO A PRINTER



Video available on how send results to a printer.

Two designated thermal printers (the Able AP1300 or the Sanibel MPT-II) are available as options and only these printers should be used. Printers supplied with the Otowave 102 are correctly configured for communication, but it is important to ensure that the correct printer is selected.

The Able and Sanibel printers have no user-settable configuration options.

Before attempting to print ensure the printer is fully charged, switched on, loaded with paper and ready to print.

To print the results of the last test select SEND TO PRINTER from the PROCESS RESULTS menu on completion of the test. (Similar facilities for printing are available from the VIEW THE LAST TEST and DATA MANAGEMENT options in the MAIN MENU.)

Press ◀ to cancel printing.

The three-character identifier for the record is printed in the “Name” field followed by the Otowave graphical displays, the analysis, and the results. The name of the hospital, the department, and the calibration dates for the instrument may also be printed if required. There is space for additional details to be handwritten by the clinician (patient name/age, operator & comments).

Thermal paper printouts can fade with exposure to light or heat. Consider transferring the data to a computer for permanent storage.

9.2. DATA TRANSFER TO NOAH OR MEDRX STUDIO

To transfer test results stored within the tympanometer to a NOAH database the NOAH Impedance module must be installed on to a computer. Alternatively, MedRx Studio allows data to be transferred to a computer and subsequently viewed, annotated & printed. This software is supplied on a USB which includes this operating manual.

Refer to the installation & operating instructions provided with the NOAH Impedance Module or MedRx Studio for further details.

If communication between the Otowave 102 and the computer cannot be established the message “Device not found” is displayed. The following points should be checked:


- Ensure the environment is suitable
- The computer has its IrDA software properly installed and the interface enabled
- If the computer has been in “Hibernate” mode, the IrDA interface is not always re-enabled; try restarting the computer
- The IrDA adapter on the computer is compatible with the Otowave
- Turn the Otowave off and on again before trying to send the data again

If communication is lost while sending the data, the message “Link was unreliable” will be displayed. Press ◀ to cancel sending the data and start the operation again.


If any other messages are displayed while sending data, turn the Otowave off and then on again and try re-sending the data. If the problem persists contact MedRx, Inc. for service.

10. DATA MANAGEMENT

Records stored in the database of the Otowave 102 can be listed, viewed, deleted, printed, or sent to a computer using the DATA MANAGEMENT option of the main menu:

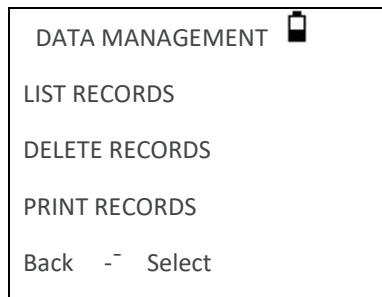

Scroll down to see the remaining choice:

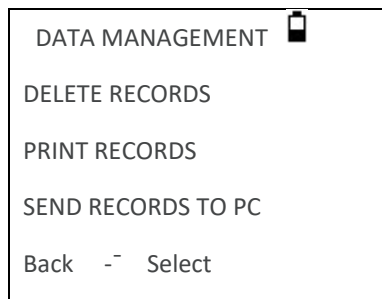

If it is required to work with the record of an individual test, select LIST RECORDS. All other options operate on groups of records.

10.1. LIST RECORDS

LIST RECORDS shows the stored tests, 6 at a time, most recent first:

Records Stored: 6/30
ABC 02/01/06 14:15 <input type="checkbox"/> <input checked="" type="checkbox"/> 2
DEF 31/12/10 09:43 <input type="checkbox"/> L
1SF 20/12/05 11:54 <input checked="" type="checkbox"/> R
MJL 17/10/05 15:48 2
AS- 17/10/05 14:22 L
BBC 12/10/05 10:24 2
Back - Select

Each entry shows:

- Three-letter patient identifier entered when the test was stored.
- Date and time of the test
- Whether the test has been printed ()
- Whether the test has been sent to a computer ()
- Whether the test is for the Left (L), Right (R) or both (2) ears

Press ▲ or ▼ to scroll through the records

Press ► to select the highlighted record

Press ◀ to return to the previous menu

When a record is selected the PROCESS RECORD menu will be displayed. This accesses the following functions:

- View the selected record
- Print the selected record
- Send the selected record to a computer
- Delete the selected record

10.2. DELETE RECORDS

DELETE RECORDS allows a group of records to be deleted. It is possible to delete all records, all records that have been printed or all records that have been sent to a computer.

Confirmation of the deletion is required.

10.3. PRINT RECORDS

PRINT RECORDS allows a group of records to be sent to the printer. It is possible to print all stored records or just those records that have not already been printed. If printing the entire database, it is recommended that a full roll of paper is loaded into the printer.


10.4. SEND RECORDS TO A COMPUTER

SEND RECORDS TO PC allows a group of records to be sent to a computer. It is possible to send all stored records or just those records that have not already been sent.

11. PERFORMING DAILY CHECKS

The operation of the Otowave 102 should be checked daily using the 4 in 1 test cavity assembly supplied with the instrument.


Select the DAILY CHECK option in the main menu:

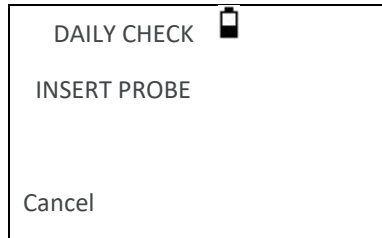

Wait until "Open" is displayed.

Insert the probe, without an ear tip, into the hole at the 2ml end of the test cavity. Make sure that the probe is pushed fully home and is held tight against the stop. The probe must be square to the end of the test cavity.

The display should show the volume of the test cavity to within ± 0.1 ml.

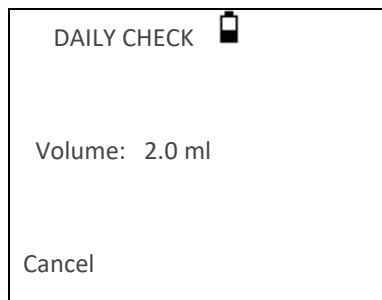

Remove the probe and repeat the test with the three remaining test cavities. The display should show the volume of the 0.2ml and 0.5ml test cavities to within ± 0.1 ml. The 5.0ml test cavity should be within ± 0.25 ml.

When the checks have been completed press ◀ to return to main menu.

12. SYSTEM INFORMATION

To review version related information of your instrument, access the start screen and use the down arrow key to move all the way to the bottom of the screen. Select System Information to find useful information such as variant of your instrument (102-1 or 102-4) and upcoming calibration dates.

1	Variant:	Instrument version (incl. version display of 102-1 or 102-4)
2	Battery:	Voltage Information
3	Last Cal:	Last calibration date
4	Next Cal:	Next calibration date
5	Serial No:	Serial number of Otowave
6	Ver.:	Firmware version
7	Date and Time:	User defined date and time

13. ROUTINE MAINTENANCE

13.1. CLEANING THE OTOWAVE

The Otowave is a precision instrument. Handle it carefully to ensure its continued accuracy and service. Before cleaning the instrument remove the batteries. Use a soft damp cloth and mild detergent to clean the instrument panel and case. Ensure no moisture enters the instrument.

13.2. EAR TIP AND PROBE

Ear tips should be replaced after a single use.

The probe tip and its associated seal are disposable devices.

The probe tip should be checked before each ear insertion to ensure it is undamaged and that none of the tubes through it are blocked. It should be replaced if necessary.

The seal should be replaced when the probe tip is replaced, if it shows signs of wear, or if a pressure leak is suspected.



WARNING

Handle the probe and accessories with care. Do not allow moisture, condensation, fluids or debris to enter the probe.

13.3. CALIBRATION AND REPAIR OF THE INSTRUMENT

MedRx recommends that the Otowave is calibrated annually. Please contact MedRx for details.

If the instrument is to be used at elevations above that specified re-calibration must be undertaken at the intended operating elevation.



WARNING

The instrument should be returned to the manufacturer for service & repair. There are no user-serviceable parts within it.

Please use the original shipping carton and packaging to transport the instrument. Place the instrument in a plastic bag before packing to prevent dirt and dust getting into the probe. Do not return the batteries with the instrument.

14. ERROR MESSAGES & FAULT CONDITIONS

If a fault condition cannot be cleared, the operator is cautioned against repeatedly starting the instrument.



PROBLEM	CAUSE	SOLUTION(S)
My profiles names are gone.	The change of the operation language will automatically default the profile names to the factory description. It is important to note that the settings of each profile stay the same.	Re-name the profile names again.
No pressure can build up and the test sequence will stay in the EQUALIZE PRESSURE SCREEN.	<ul style="list-style-type: none"> • No seal can be obtained • Estimated volume is too high (perforated ear drum) • Wrong ear tip size chosen • Probe is blocked 	<ul style="list-style-type: none"> • Examine the probe tip for contamination and replace the probe tip • Reposition the probe • Change the ear tip
No reflex test is conducted after the tympanometry even though the reflex test is active in the REFLEX SEQUENCE.	In REFLEX SELECTION the setting is set to ONLY IF PEAK IS FOUND or NEVER MEASURE .	Change settings in REFLEX SELECTION to desired option.
Last measured data cannot be found under VIEW THE LAST TEST.	NEW TEST might have been selected in between and thereby deleted the last test(s) from the short-term memory.	To be stored data should be stored immediately.
BLOCKED PROBE Indicator LED a and b flash fast.	<ul style="list-style-type: none"> • Probe is blocked • Probe placed against ear canal skin • Probe disconnected from base unit 	<ul style="list-style-type: none"> • Examine the probe tip for contamination and replace the probe tip • Reposition the probe • Change the ear tip • Check probe connection with base unit
WITHDRAW PROBE Indicator LED a and b flash fast.	<ul style="list-style-type: none"> • The probe has been moved during measurement. • Test has been started with the probe already inserted into the ear. 	Reposition the probe
Volume outside range WITHDRAW PROBE Indicator LED a and b flash fast.	<ul style="list-style-type: none"> • Ear canal volume is > 5ml. • Probe is not properly inserted into the ear. 	Reposition the probe

PROBLEM	CAUSE	SOLUTION(S)
Pressure lost WITHDRAW PROBE Indicator LED a and b flash fast.	<ul style="list-style-type: none"> • Ear seal has been broken while testing for seal. 	<ul style="list-style-type: none"> • Reposition the probe
Measurement timed out Indicator LED a and b flash fast.	<ul style="list-style-type: none"> • Occurs when the ear seal check is set to EXTENDED • Pump failed to achieve the starting pressure within 4 s. • Pressure failed to reach -400 daPa within 12 s. 	<ul style="list-style-type: none"> • Reposition the probe. Retry the test. If the problem persists, contact your MedRx service centre.
VOLUME OUTSIDE RANGE Indicator LED a and b flash.	<ul style="list-style-type: none"> • Probe not placed correctly in ear canal. 	<ul style="list-style-type: none"> • Reposition probe.
PROBE NOT CLEAR Indicator LED b steady light.	<ul style="list-style-type: none"> • Probe is blocked Probe placed incorrectly 	<ul style="list-style-type: none"> • Check that the probe is not inserted into a test cavity at start-up. Please ensure the probe is not blocked or obstructed.
AIRFLOW ERROR Indicator LED b steady light.	Fault with air system and/or pump. Cannot determine pump direction.	Unknown pump fault. Restart the unit. If problem persists, contact your MedRx service center.
AIRFLOW ERROR RESTART THE UNIT Indicator LED b steady light.	Fault with air system and/or pump.	Restart the unit. If problem persists, contact your MedRx service center.
WARNING! CALIBRATION EXPIRED Indicator LED b steady light.	The current date is later than the next calibration date. Check that the clock is set to the correct date. If so, arrange for the instrument to be recalibrated. Tests can still be performed.	Recalibration needed before ..\Desktop\TYMP-102-Manual-Cover-and-inside-cover-page.pdf further tests are performed.
WARNING! DEVICE UNCALIBRATED. Indicator LED b steady light.	One or more default values require recalibration before further tests are performed.	Contact your MedRx service center.
WARNING! DEFAULTS RELOADED. Indicator LED b steady light.	Default configuration settings reloaded.	Default configuration settings reloaded. If the error persists, contact your MedRx service center.
Printing Error No connection can be established with the printer	<ul style="list-style-type: none"> • Printer is switched off or not charged • Connection between printer and base unit cannot be established. 	<ul style="list-style-type: none"> • Restart the base unit • Restart the printer • Charge printer • Ensure the connection between printer and base unit is established.

If difficulties resolving fault conditions occur the equipment distributor (or MedRx if purchased directly) should be consulted.

15. TECHNICAL SPECIFICATION

15.1. PERFORMANCE

Tympanometry	
Instrument type	Meatus compensated tympanometer
Analysis performed	Compliance peak level (in ml) & pressure; Gradient (in daPa); Ear Canal Volume (ECV) @ 200 daPa
Probe tone levels and accuracy	226Hz +/- 2%; 85dB SPL +/-2dB over range 0.2ml to 5ml
Pressure levels and accuracy	+200daPa to -400daPa +/-10daPa or +/-10% (whichever is larger) over range
Ear volume measurement range and accuracy	0.2ml to 5ml +/- 0.1ml or +/-5% (whichever is larger) over entire range
Sweep speed	Typically, 200-300daPa/sec; dependent on ear/cavity volume
Pressure limits (safety cut-out)	+600 to -800 daPa
Number of samples stored	100 per tympanogram
Reflex measurements	
Measurement mode	Ipsilateral
Reflex tone levels and accuracy (Referenced to 2ml calibration volume - compensates for measured ear volume)	102-1: 1kHz (+/-2%) 102-4: 500Hz,1kHz,2kHz,4kHz (+/-2%) Configurable over range 70dB to100dBHL +/-3dB (4kHz restricted to 95dBHL)
Number of reflex levels	Four: 100dB with 5dB or 10 dB steps; 95dB, 90dB or 85dB with 5 dB steps
Reflex analysis	Reflex pass/fail at each level tested; maximum amplitude of each reflex; nominal pressure used for the reflex test (computer display only)
Pressure used for reflex measurement	Pressure at tympanogram peak, or at 0daPa (if no peak found)
Reflex stimulus control	Stimulus presented at all levels, or stimulus ceases when a reflex is found
Reflex detection threshold and accuracy	0.01ml to 0.5ml +/-0.01ml (configurable in 0.01ml steps)
Reflex tone duration	0.6 seconds
Number of records stored in Patient Database	32
Data storage	Any recording can be stored once the tympanogram is viewed. Patient Initials (A-Z, 0-9, "-") must be entered before storage.
Data held	Patient Initials, Tympanogram and Reflex graphs and analysis for Left Ear and/or Right Ear, Time and Date of recording, which ears were tested, whether or not the record has been printed and/or sent to a computer, parameters used for analysis, 128 bit Globally Unique Identifier (GUID)
Display mode	Records listed in reverse chronological order (latest first), with indication of data stored as described above
Real Time Clock	
Time stamps	Time and date stamp applied to all recordings, and to the last calibration date
Backup power supply	> 30 days without main batteries fitted

Languages	
Operating Languages	English, German, French, Spanish, Portuguese, or Italian
Printing	
Supported printer	Sanibel MPT-II or Able AP1300
Interface	Infra-red, IrDA hardware, 9600 baud
Information printed	Tympanogram, Tympanogram analysis parameters, Reflex graphs, Reflex analysis parameters, Serial Number of device, Last and Next Due Calibration dates; space for patient & clinician's details to be entered.
Serial Interface to computer	
Interface	OBEX (Object Exchange) service running on top of IrDA stack. Auto-selects between 9600-115200 baud.
Information sent	Patient header, left and right ear data.
Power Supply	
Battery Types	4 AA cells; either Alkaline (1.5V nominal) or NiMH rechargeable (1.2V nominal, which must be 2.3 Ah capacity or greater).
Warm-up period	None at room temperature
Number of recordings from one set of cells	Approx. 200 (Alkaline) or 100 (NiMH)
Auto power-off delay	90 or 180 seconds
Idle current	70mA
Current while testing	230mA
Physical	
Display	128 x 64 pixels / 8 lines of 21 characters
Dimensions	190mm long x 80mm wide x 40mm high excluding probe 210mm long including probe
Weight (without batteries)	285 g
Weight (with batteries)	380 g
Environmental	
Operating temperature range	+15°C to +35°C
Operating humidity range	30% to 90% RH, non-condensing
Operating atmospheric pressure range	980 to 1040 mb
Transport and storage temperature range	-20°C to +70°C
Transport and storage humidity range	10% to 90% RH, non-condensing

Transport and storage atmospheric pressure range	900 to 1100 mb
Standards conformance	
Safety	IEC 60601-1(plus UL, CSA & EN deviations)
EMC	IEC 60601-1-2
Performance	IEC 60645-5, Type 2 Tympanometer ANSI 3.39, Type 2
CE mark	To the EU Medical Device Regulation

15.2. EQUIPMENT CLASSIFICATION

Type of protection against electric shock	Internally Powered
Degree of protection against electric shock	Type BF applied part
Degree of protection against ingress of water	Not protected
Mode of operation	Continuous operation
Equipment mobility	Portable

The Otowave 102 Tympanometer is classified as a Class IIa device under Annex VIII of the EU Medical Devices Regulation.

15.3. SYMBOLS



Definition: Identifies the control by means of which the instrument is switched on from (or returned to) a standby condition.



Definition: Refer to instruction manual (mandatory)



Definition: Type BF applied part – an applied part providing a higher degree of protection against electric shock than that provided by a Type B applied part, particularly regarding allowable patient leakage current and patient auxiliary current.

The applied part is the ear tip.



Definition: Date of Manufacture



Definition: Manufacturer



Definition: Medical product

16. ORDERING CONSUMABLES AND ACCESSORIES

To order consumables, additional accessories and to replace detachable parts that have been damaged, please contact the manufacture for current prices and delivery charges.

17. DISPOSAL INFORMATION



The manufacturer is fully compliant with the WEEE (Waste Electrical and Electronic Equipment) Regulations. Our PRN (Producer Registration Number) is WEE/GA0116XU and we are registered with the approved WEEE Compliance Scheme, B2B Compliance, approval number WEE/MP3338PT/SCH.

The main purpose of the WEEE Regulations is to encourage the segregation of waste electrical items from the general waste stream and into reuse, recovery, and recycling routes.

Therefore, for any waste electrical units purchased from manufacturer that either:

- bear the crossed out wheeled bin symbol with black bar underneath, or
- have been replaced with new products on a like-for-like basis

please contact manufacturer WEEE Compliance Scheme, B2B Compliance, using the details below. B2B Compliance will be able to provide further information on how to recycle your waste electrical units and answer any queries you may have.

B2B Compliance

Tel: +44 (0) 1691 676 124 (Option 2)

Email: operations@b2bcompliance.org.uk

18. EMC GUIDANCE & MANUFACTURER'S DECLARATION

Guidance and manufacturer's declaration – electromagnetic emissions		
The Otowave 102 Tympanometer is intended for use in the electromagnetic environment specified below. The customer or user of the Otowave 102 Tympanometer should assure that it is used in such an environment.		
Emissions test	Compliance	Electromagnetic environment – guidance
RF emissions CISPR 11	Group 1	The Otowave 102 Tympanometer uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause interference in nearby electronic equipment. The Otowave 102 Tympanometer is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
RF emissions CISPR 11	Class B	
Harmonic emissions IEC 61000-3-2	Not applicable	
Voltage fluctuations/flicker emissions IEC 61000-3-3	Not applicable	


Guidance and manufacturer's declaration – electromagnetic immunity (1)			
The Otowave 102 Tympanometer is intended for use in the electromagnetic environment specified below. The customer or user of the Otowave 102 Tympanometer should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment – guidance
Electrostatic Discharge (ESD) IEC 61000-4-2	±8 kV contact ±15 kV air	±8 kV contact ±15 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/output lines	Not applicable	
Surge IEC 61000-4-5	±1 kV differential mode ±2 kV common mode	Not applicable	Not applicable

EMC GUIDANCE & MANUFACTURER'S DECLARATION

Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment – guidance
Voltage dips, short interruptions, and voltage variations on power supply input lines IEC 61000-4-11	<5% U_T (>95% dip in U_T) for 0.5 cycle 40% U_T (60% dip in U_T) for 5 cycles 70% U_T (30% dip in U_T) for 25 cycles <5% U_T (>95% dip in U_T) for 5 sec	Not applicable	Not applicable
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	30 A/m	30 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.
NOTE: U_T is the a.c. mains voltage prior to the application of the test level			

Guidance and manufacturer's declaration – electromagnetic immunity (2)

The Otowave 102 Tympanometer is intended for use in the electromagnetic environment specified below. The customer or user of the Otowave 102 Tympanometer should assure that it is used in such an environment.

Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment – guidance
Radiated RF IEC 61000-4-3	10 V/m 80MHz to 2.7GHz	10 V/m 80MHz to 2.7GHz	<p>Portable and mobile RF communications equipment should be used no closer to any part of the Otowave 102 Tympanometer, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.</p> <p>Recommended separation distance</p> <p>$d = 1.2\sqrt{P}$ 80MHz to 800MHz</p> <p>$d = 2.3\sqrt{P}$ 800MHz to 2.5GHz</p> <p>where P is the maximum output power rating of the transmitter in Watts (W) according to the transmitter manufacturer and d is the recommended separation distance in metres (m).</p> <p>Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey,^a should be less than the compliance level in each frequency range.^b</p> <p>Interference may occur in the vicinity of equipment marked with the following symbol:</p> <div style="text-align: center;">  </div>

NOTE 1 At 80MHz and 800MHz, the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

NOTE 3 WARNING: Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30cm (12 inches) to any part of the Otowave 102 Tympanometer including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.

Guidance and manufacturer's declaration – electromagnetic immunity (2)			
a	Field strength from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the Otowave 102 Tympanometer is used exceeds the applicable RF compliance level above, the Otowave 102 Tympanometer should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the Otowave 102 Tympanometer.		
b	over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.		
Recommended separation distances between portable and mobile RF communications equipment and the Otowave 102 Tympanometer			
The Otowave 102 Tympanometer is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the Otowave 102 Tympanometer can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the Otowave 102 Tympanometer as recommended below, according to the maximum output power of the communications equipment.			
Rated maximum output power of transmitter W	Separation distance according to frequency of transmitter m		
	150 kHz to 80 MHz d = 1.2√P	80 MHz to 800 MHz d = 1.2√P	800 MHz to 2.5 GHz d = 2.3√P
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23
For transmitters rated at a maximum output power not listed above, the recommended separation distance d in metres (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in Watts (W) according to the transmitter manufacturer.			
NOTE 1 At 80MHz and 800MHz, the separation distance for the higher frequency range applies.			
NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.			

19. USE WITH NON-MEDICAL ELECTRICAL EQUIPMENT

Any person who connects external equipment to signal input, signal output or other connectors has created a medical electrical system and is therefore responsible for the system complying with the requirements of clause 16 of IEC 60601-1:2005 (*General requirements for basic safety and essential performance*).

If connections are made to standard equipment such as printers and computers, special precautions must be taken in order to maintain medical safety. The following notes are provided for guidance in making such connections to ensure that the general requirements of clause 16 of IEC 60601-1:2005 are met.

The Otowave 102 tympanometer uses an industry-standard infra-red means of communication (an IrDA port) in order to reduce any potential hazard associated with the use of mains-powered equipment connecting to this interface.


External equipment intended for connection to signal input, signal output or other connectors, shall comply with the relevant IEC or international standards (e.g. IEC 60950, CISPR 22 & CISPR 24 for IT equipment, and the IEC 60601 series for medical electrical equipment).

Equipment not complying with IEC 60601 shall be kept outside the patient environment, as defined in IEC 60601-1:2005 (at least 1.5m from the patient).

The operator must not touch the connected equipment and the patient at the same time as this would result in an unacceptable hazard.

Refer to Diagrams 1 & 2 below for typical configurations of connected peripheral equipment.

Refer to the manufacturer at the address given on the front of this user manual if advice is required regarding the use of peripheral equipment.

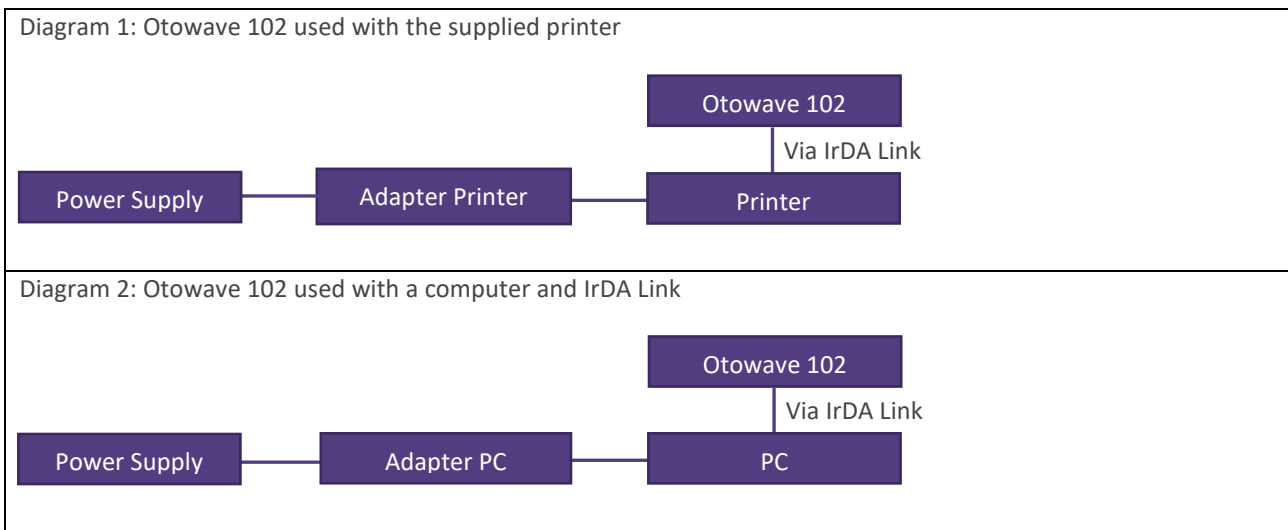

Copyright © 2021 MedRx Inc.

All rights reserved. No part of this publication may be reproduced or transmitted in any form or by any means without the prior written permission of MedRx Inc.