Instructions for use



BTE PP BTE

Oticon Opn™ Oticon Opn S™ Oticon Opn Play™ Oticon Siya





Model overview

This booklet is valid for Oticon Opn™, Oticon Opn S™, Oticon Opn Play™, and Oticon Siya families, in the following hearing aid models:

Oticon Opn FW6 ☐ Oticon Opn 1 BTE13 PP ☐ Oticon Opn 2 BTE13 PP ☐ Oticon Opn 3 BTE13 PP	GTIN: (01) 05707131335227 GTIN: (01) 05707131335234 GTIN: (01) 05707131335241
Oticon Opn S FW7 ☐ Oticon Opn S 1 BTE PP ☐ Oticon Opn S 2 BTE PP ☐ Oticon Opn S 3 BTE PP	GTIN: (01) 05707131349811 GTIN: (01) 05707131349828 GTIN: (01) 05707131349835
Oticon Opn Play FW7 ☐ Oticon Opn Play 1 BTE PP ☐ Oticon Opn Play 2 BTE PP	GTIN: (01) 05707131349842 GTIN: (01) 05707131349859

Oticon Siya FW1 □ Oticon Siya 1 BTE PP GTIN: (01) 05707131340887 □ Oticon Siya 2 BTE PP GTIN: (01) 05707131340894 □ Oticon Siya 1 BTE GTIN: (01) 05707131340887 □ Oticon Siya 2 BTE GTIN: (01) 05707131340894

☐ LED light for visual indication. Not available for Oticon Siya.

The LED light is used to help, caregivers, parents, and teachers to operate the hearing aid and to give instructions on relevant functions and modes (see relevant information throughout the booklet).

Introduction to this booklet

This booklet gives you guidance on how to use and maintain your new hearing aid. Please read the booklet carefully, including the **Warnings** section. This will help you to get the most out of your new hearing aid.

Your hearing care professional has adjusted the hearing aid to meet your needs. If you have additional questions, please contact your hearing care professional.

| About | Start-up | Handling | Options | Tinnitus | Warnings | More info |

For your convenience, this booklet contains a navigation bar to help you easily navigate through the different sections.

Intended use Oticon Opn, Oticon Opn S, and Oticon Siya

The hearing aid is intended to amplify and transmit sound to the ear, and thereby compensating for impaired hearing within mild to severe-to-profound hearing loss.

Intended use Oticon Opn Play

The hearing aid is intended to amplify and transmit sound to the ear, and thereby compensate for impaired hearing within mild to severe hearing loss. This hearing aid is intended for use by infants, children and adolescents/young adults.

IMPORTANT NOTICE

The hearing aid amplification is uniquely adjusted and optimized to your personal hearing capabilities during the hearing aid fitting performed by your hearing care professional.

Table of contents

About		
	Your hearing aid and earpiece	17
	Identify left and right hearing aid	10
	MultiTool for handling of batteries and cleaning	1
Start-up		
	Turn the hearing aid on and off	18
	When to replace the battery	19
	How to replace the battery (size 13)	20
Handling		
	Put on the hearing aid with sound hook	2
	Caring for your hearing aid	2
	Clean the earmold	24
	Put on hearing aid with thin tube	20
	Clean the thin tube	2
	Replace standard earpieces	28
	Clean customized earpieces	30

Table of contents

	Replace ProWax filter	31
	Flight mode	32
Options		
	Optional features and accessories	33
	Change program	34
	Change volume	36
	Mute	38
	Use hearing aid with iPhone and iPad	39
	Pair with iPhone	40
	Wireless accessories	42
	Other options	44
	Tamper-resistant battery drawer	46
	Sound and LED indications	48
Tinnitus		
	Tinnitus SoundSupport™ (optional)	52
	Guidelines for tinnitus sound generator users	53


	Sound and volume adjustment	5
	Limitation on use time	5
	Tinnitus SoundSupport warnings	6
Varnings	-	
	General warnings	6
lore info		
	Troubleshooting	7
	Water and dust resistant (IP68)	7
	Conditions of use	7
	Warranty	7-
	Mobile phone	7
	Technical information	7
	Your individual hearing aid settings	8
	Technical Data	8


Your hearing aid and earpiece

There are two different attachments and several different earpieces available for the hearing aid.

□ With sound hook and earmold earpiece

With thin tube (Corda miniFit)





The thin tube uses one of the following earpieces:

Standard earpieces:



☐ Open dome



 \square Bass dome, single vent



☐ Bass dome, double vent



☐ Power dome



☐ Grip Tip

Available in small and large, left and right, with or without vent.

10 mm

12 mm

Dome sizes



Customized earpieces:



☐ MicroMold



☐ LiteTip



☐ VarioTherm® MicroMold




☐ VarioTherm® LiteTip


® VarioTherm is a registered trademark of Dreve

Please see details for replacing the dome in chapter "Replace dome or GripTip"

With sound hook and earmold

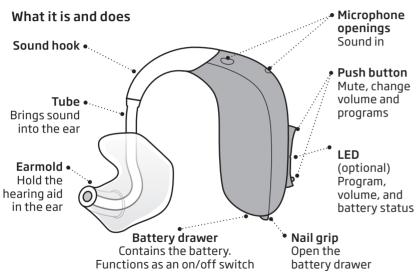


With thin tube

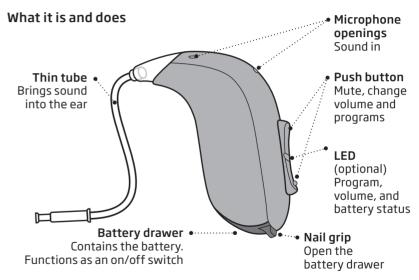

Identify left and right hearing aid


It is important to distinguish between the left and the right hearing aid as they may be programmed differently.

You can find left/right color indicators in the battery drawer. Indicators can also be found on MicroMolds (optional).

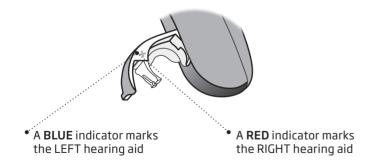

MultiTool for handling of batteries and cleaning

The MultiTool contains a magnet that makes it easier to replace the battery in the hearing aid. It also contains a brush and wire loop for cleaning and removing earwax. If you need a new MultiTool, please contact your hearing care professional.



IMPORTANT NOTICE

Your MultiTool has a built-in magnet. Keep the MultiTool at least 12 in. away from credit cards and other magnetically sensitive devices.

Turn the hearing aid on and off

The battery drawer is also used to switch the hearing aid on and off. To save battery life, make sure your hearing aid is switched off when you are not wearing it. If you wish to return to the standard settings of the hearing aid, simply open and close the battery drawer (quick reset).

Optional LED

Two long green blinks indicate that the hearing aid is turned on.

Turn ON Close the battery drawer with the battery in place.





Turn OFF Open the battery drawer.



When to replace the battery

When it is time to replace the battery, you will hear three beeps repeated in moderate intervals until the battery runs out.





Battery tip

To make sure the hearing aid is always working, bring spare batteries with you, or replace the battery before you leave home.

Optional LED

Red blinks, continuously repeated, to indicate battery low.

^{*} Bluetooth® will be turned off and it will not be possible to use wireless accessories. Note: Batteries need to be replaced more often if you are streaming to your hearing aid.

How to replace the battery (size 13)

1. Remove



Fully open the battery drawer. Remove the battery.

2. Uncover



Remove the sticky label from the + side of the new battery.

Tip: Wait 2 minutes so that the battery can draw air, to ensure optimal functioning.

3. Insert



Insert the new battery into the battery drawer. Insert it from above, NOT from the side.

Make sure the + side is facing up.

4. Close



Close the battery drawer. The hearing aid will play a jingle through the earpiece.

Hold the earpiece close to your ear to hear the jingle.

Tip



The MultiTool can be used to change the battery. Use the magnetic end to remove and insert batteries.

The MultiTool is provided by your hearing care professional.

Put on the hearing aid with sound hook

Read the following pages if you have a hearing aid with a sound hook and earmold.



The earmold is customized for you and fits your ear shape. The earmolds are unique for the left or the right ear.

Step 1



Gently pull your ear outwards and press the earmold in the direction of the ear canal, twisting slightly.

Step 2



Place the hearing aid behind your ear.

Caring for your hearing aid

When handling your hearing aid, hold it over a soft surface to avoid damage in case you drop it.

Clean the microphone openings Carefully brush any debris away from the openings. Gently brush the surface. Make sure the brush is not pressed into the openings.



IMPORTANT NOTICE

Use a soft, dry cloth to clean the hearing aid. The hearing aid must never be washed or immersed in water or other liquids.

Clean the earmold

The earmold should be cleaned regularly. Use a soft cloth to clean the surface of the earmold. Use the MultiTool wire loop to clean the opening.

Replace the tube

The tubing between the earmold and the hearing aid should be replaced if it becomes yellow or stiff. Consult your hearing care professional about this.



Wash the earmold

Step 1



Make sure you are able to identify which earmold is for which hearing aid before disconnecting them from the hearing aid.

Step 2



Disconnect the tube and earmold from the hook. Hold the hook firmly when pulling it off the tube. Otherwise the hearing aid may be damaged.

Step 3



Wash the earmold and tube using mild soap. Rinse and dry completely before reconnecting to the hearing aid.

Put on hearing aid with thin tube

Read the following pages if your hearing aid has a thin tube.

Step 1



Place the hearing aid behind your ear.

The thin tube should only be used with an attached earpiece. Use only parts designed for your hearing aid.

Step 2



Hold the bend of the tube between your thumb and index finger. The earpiece should point towards the ear canal opening.

Step 3




Gently push the earpiece into your ear canal until the thin tube sits close to your head. If the thin tube has an ear grip, place it in the ear so it follows the contour of the ear.

Clean the thin tube

The thin tube should be cleaned to keep it clear of moisture and wax. If not cleaned, it may become blocked with wax, which stops sound from coming into your ear.

Step 1



Pull the thin tube out of the hearing aid.

Step 2



Push the cleaning tool all the way through the thin tube.


Step 3




Reconnect the thin tube to the hearing aid.

Replace standard earpieces


The standard earpiece (dome or Grip Tip) should not be cleaned. If the earpiece is filled with wax, replace it with a new one. Grip Tips should be replaced at least once a month.



Hold on to the end of the thin tube and then pull off the earpiece.



Insert the thin tube exactly into the middle of the earpiece to obtain a secure attachment.



Push firmly to ensure that the earpiece is fastened securely.


IMPORTANT NOTICE

If the earpiece is not on the thin tube when removed from the ear, the earpiece may still be in the ear canal. Consult your hearing care professional for further instructions.

Clean customized earpieces

The earpiece should be cleaned regularly. The earpiece has a white wax filter*that keeps wax and debris from damaging the hearing aid.

Replace the filter when clogged, or if the sound is not normal, or contact your hearing care professional.




IMPORTANT NOTICE

Always use the same type of wax filter as was originally supplied with the hearing aid. If you are in any doubt about the use or replacement of wax filters, contact your hearing care professional.

Replace ProWax filter

1. Tool



Remove the tool from the shell. The tool has two pins, one empty for removal and one with the new wax filter.

2. Remove



Push the empty pin into the wax filter in the earpiece and pull it out.

3. Insert



Insert the new wax filter using the other pin, remove the tool, and throw it out.


^{*} VarioTherm MicroMold and LiteTip do not have a wax filter

Flight mode

When flight mode is activated, Bluetooth® is turned off. The hearing aid will still be working. Pressing the push button on one hearning aid will activate flight mode on both hearing aids.

Optional LED

The LED will blink green, red, and red a few times. This confirms that flight mode is activated.



To activate and deactivate Press the push button for at least 7 seconds. An audible jingle confirms your action.

Opening and closing the battery drawer will also deactivate flight mode.

Optional features and accessories

The features and accessories described in the following pages are optional. Please contact your hearing care professional to find out how your hearing aid is programmed.

If you experience difficult listening situations, a special program may be helpful. These are programmed by your hearing care professional.

Write down any hearing situations in which you may need help.

Change program

Your hearing aid can have up to 4 different programs. These are programmed by your hearing care professional.

Optional LED

The number of green blinks indicate the selected program.



Press up or down between programs.

Note that you can change continuously between programs - both up and down in the program order. For example, if you want to go from program 1 to 4, you can press the down button once instead of pressing the up button 3 times.


To be filled out by the hearing care professional

Program	Activat	ion sound	When to use
1)	"1 beep"	
2	7,7	"2 beeps"	
3	الرار	"3 beeps"	
4	תתתת	"4 beeps"	

Program change:	□LEFT	□RIGHT	☐ Short press	□ Long press
-----------------	-------	--------	---------------	--------------

☐ Change volume

The push button allows you to adjust the volume. You will hear a click when you turn the volume up or down.

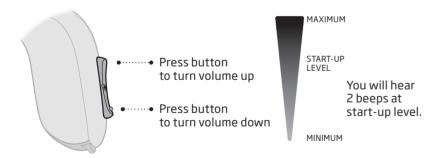

Optional LED

The LED will blink green to confirm changes in volume, and a long green blink at start-up level. The LED will show a red blink when the volume reaches the minimum or maximum level.

To be filled out by the hearing care professional

Volume change □ LEFT	□RIGHT	□Short press	
----------------------	--------	--------------	--

Mute

Use the mute function if you need to silence the hearing aid. The mute function only mutes the microphone(s) on the hearing aid.

Optional LED

Green and red blinks, continuously repeated, to indicate mute.



Apply a long press (4 seconds) to either end of the button to mute the hearing aid.

To reactivate the hearing aid, push the button briefly.

IMPORTANT NOTICE

Do not use the mute function as an off switch, as the hearing aid still draws current from the battery in this mode.

Use hearing aid with iPhone and iPad

Your hearing aid is Made for iPhone® and allows for direct communication and control with iPhone, iPad® or iPod touch®. For assistance in using these products with your hearing aid, please contact your hearing care professional or visit: www.oticon.com/support.



For information on compatibility, please visit www.oticon.com/support.

Use of the Made for Apple badge means that an accessory has been designed to connect specifically to the Apple product(s) identified in the badge, and has been certified by the developer to meet Apple performance standards. Apple is not responsible for the operation of this device or its compliance with safety and regulatory standards.

Please note that use of this Accessory with iPod, iPhone, or iPad may affect wireless pelformance.

Apple, the Apple logo, iPhone, iPad, and iPod touch are trademarks of Apple Inc., registered in the U.S. and other countries.

Pair with iPhone

1. Settings



Open your iPhone and go to "Settings". Make sure Bluetooth is on. Then choose "General".

2. General



On the "General" screen, choose "Accessibility".

3. Accessibility



On the "Accessibility" screen, choose "MFi Hearing Devices".

4. Prepare





Open and close the battery drawer on both hearing aids, and place them close to your iPhone. The hearing aids remain in pairing mode for 3 minutes.

5. Select



Your iPhone will detect the hearing aids for pairing. Detected devices will appear in your iPhone list. Choose your hearing aids.

6. Confirm pairing



Confirm pairing. If you have two hearing aids, pairing confirmation is needed for each hearing aid.

41

Wireless accessories

As an enhancement to your wireless hearing aids, a range of accessories is available. These can enable you to hear and communicate better in many everyday situations.

☐ ConnectClip

When paired with your mobile phone, you can use the hearing aid as a hands-free headset; ConnectClip can also be used as a remote microphone.

☐ TV Adapter 3.0

Wireless transmitter of sound from TV and electronic audio devices. TV Adapter streams sound directly to your hearing aid.

\square FM

Your hearing aid supports the option of attaching an FM receiver. The FM system allows you to receive speech or audio signals directly to your hearing aid from a dedicated transmitter.

☐ Remote Control 3.0

Offers the ability to change program, adjust volume, or mute your hearing aid.

☐ Phone Adaptor 2.0

Connects your traditional home phone to the ConnectClip via Bluetooth allowing for handsfree phone calls.

☐ Oticon ON App

Offers an intuitive and discreet way to control your hearing aid. For iPhone, iPad, iPod touch, and Android™ devices.

For more information visit www.oticon.com/support or contact your hearing care professional.

Other options



☐ Telecoil program

Telecoil helps you hear better when using a telephone with a built-in loop, or when you are in buildings with teleloop systems such as theaters, houses of worship, or lecture rooms. This symbol or a similar sign is shown wherever a teleloop has been installed.



☐ Auto Phone - optional for Oticon Opn and Oticon Siya

The Auto Phone can automatically activate a phone program in the hearing aid, if you place a dedicated magnet on your phone.

☐ Direct Audio Input (DAI)

DAI allows your hearing aid to receive signals directly from external sources such as TV, radio, music players, etc. The DAI adaptor is attached to your hearing aid and then connected via a cable to the external sound source.

For more information, please contact your hearing care professional.

IMPORTANT NOTICE

Only connect hearing aids with DAI to electrically powered devices that comply with EN 60950-1, EN 60065 or equivalent safety standards. The external signal source determines the safety of hearing aids with DAI.

Tamper-resistant battery drawer

To keep the battery out of reach of infants, small children, and people with cognitive impairments, a tamper-resistant battery drawer should be used.

IMPORTANT NOTICE

Avoid excessive force when opening the battery drawer in the locked position. Do not force the battery drawer beyond its fully opened position. Make sure to insert the battery correctly.

Please contact your hearing care professional if you suspect the tamper-resistant effectiveness or locking ability is damaged.

To lock the battery drawer



Close the battery door completely and make sure it is locked.

Tool to unlock the battery drawer



Use this small blue tool provided by your hearing care professional.

Unlock the battery drawer



Insert the tip of the blue tool into the small hole at the back of the battery drawer.

- 1. Move it to the right and push up
- 2. Open the battery drawer

Sound and LED indications

Different sound and LED light indications help to show the hearing aid status. The different setting options are listed on the following pages.

Your hearing care professional can set sound and LED indications to match your preferences.

Program status	Sound	LED	LED comments
Program 1	1 beep	0	
Program 2	2 beeps	00	
Program 3	3 beeps	000	Continuously repeated
Program 4	4 beeps	0000	
Wireless accessories	2 beeps		or repeated 3 times with small pauses
Wireless accessories incl. microphone	2 beeps		
Flight mode	Sound	LED	
Flight mode active	4 beeps	000	
Flight mode inactive	4 beeps		

Green, short blink Green, long blink Red, short blink

On	Sound	LED	LED comments
On	Start-up jingle		Shown one time
Volume	Sound	LED	
Preferred volume	☐ 2 beeps		
Minimum / maximum volume	☐ 3 beeps		Shown one time
Volume up / down	☐ 1 beep		
Mute			Continuously repeated or repeated 3 times with small pauses
Green, short blink	Green, long blink	Red, short blink	

Warnings	Sound	LED	LED comments
Battery low indication	☐ 3 beeps		Continuously repeated
Battery shut down	4 descending tones		
Microphone service check needed	8 beeps repated 4 times		Repeated 4 times with small pauses

Red, short blink Red, long blink

☐ Tinnitus SoundSupport™ (optional)

Intended use of Tinnitus SoundSupport

Tinnitus SoundSupport is a tool intended to generate sounds to provide temporary relief for patients suffering from tinnitus as part of a tinnitus management program.

The target population is the adult population (over 18 years old).

Tinnitus SoundSupport is targeted to licensed hearing care professionals (audiologists, hearing aid specialists, or otolaryngologists) who are familiar with the evaluation and treatment of tinnitus and hearing loss. Fitting of Tinnitus SoundSupport must be done by a hearing care professional participating in a tinnitus management program.

Guidelines for tinnitus sound generator users

These instructions contain information about Tinnitus SoundSupport, which may have been enabled in your hearing aids by your hearing care professional.

Tinnitus SoundSupport is a tinnitus management device intended to generate sound of sufficient intensity and bandwidth to help manage tinnitus.

Your hearing care professional will also be able to offer the appropriate follow-up care. It is important to follow his/her advice and directions regarding such care.

Prescription use only

Good health practice requires that a person reporting tinnitus have a medical evaluation by a licensed ear physician before using a sound generator. The purpose of such an evaluation is to ensure that any medically treatable condition that may cause tinnitus is identified and treated prior to using a sound generator.

Sound and volume adjustment

Tinnitus SoundSupport is programmed by your hearing care professional to match your hearing loss and preferences for tinnitus relief. It offers a number of different sound options. Together with your hearing care professional, you can select your preferred sound(s).

Tinnitus SoundSupport programs

Together with your hearing care professional, you can decide for which programs you may want to have Tinnitus SoundSupport activated. The sound generator can be activated in up to four different programs.

Mute

If you are in a program for which Tinnitus SoundSupport is activated, the mute functionality will mute only the environmental sounds, and not the sound from Tinnitus SoundSupport. See chapter: "Mute the hearing aid".

Volume adjustments with Tinnitus SoundSupport

When you select a hearing aid program for which Tinnitus SoundSupport is activated, your hearing care professional can only set the push button on your hearing aid to work as a volume control for the tinnitus relief sound.

Your hearing care professional will set the volume control for the sound generator in one of two ways:

- A) Change volume in each ear separately or
- B) Change volume in both ears simultaneously.

A) How to change Tinnitus SoundSupport volume in each ear separately To increase volume (on one hearing aid only), use a short press on the upper part of the push button repeatedly until desired level is reached. To decrease volume (on one hearing aid only), use a short press on the lower part of the push button repeatedly until desired level is reached.
B) How to change Tinnitus SoundSupport volume in both ears simultaneously You can use one hearing aid to increase/decrease the sound in both hearing aids. When changing the volume in one hearing aid, the volume on the other hearing aid will follow. To increase volume, use a short press on the upper part of the push button repeatedly. To decrease volume, use a short press on the lower part of the push button repeatedly.

To be filled out by your hearing care professional.

Limitation on use time

Daily use

The volume levels of Tinnitus SoundSupport can be set to a level which could lead to permanent hearing damage when used for a prolonged period of time. Your hearing care professional will advise you of the maximum amount of time per day you should use Tinnitus SoundSupport. It should never be used at uncomfortable levels.

See table "Tinnitus SoundSupport: Limitation on use" in section "Your individual hearing aid settings" at the end of this booklet to learn how many hours per day you can safely use the relief sound in your hearing aids.

Important information for hearing care professionals about Tinnitus SoundSupport

Device description

Tinnitus SoundSupport is a module function that can be enabled in the hearing aids by a hearing care professional.

Maximum wearing time

The wearing time of Tinnitus SoundSupport will decrease as you increase the level above 80 dB(A) SPL. The fitting software will automatically display a warning when the hearing aid exceeds 80 dB(A) SPL. See "Max wearing time indicator" next to the tinnitus fitting graph in the fitting software.

The volume control is deactivated

By default, the volume control for the sound generator is deactivated in the hearing aid. Risk of noise exposure increases when the volume control is activated.

If the volume control is activated

A warning may be displayed if you activate the tinnitus volume control in the "Buttons & Indicators" screen. This occurs if the relief sound can be listened to at levels that may cause hearing damage. The "Max wearing time" table in the fitting software displays the number of hours the patient can safely use Tinnitus SoundSupport.

- Note the max wearing time for each program for which Tinnitus SoundSupport is activated.
- Write those values in the table "Tinnitus SoundSupport: Limitation on use", found in the back of this booklet.
- Instruct your patient accordingly.

⚠ Tinnitus SoundSupport warnings

If your hearing care professional has activated the sound generator Tinnitus SoundSupport, please pay attention to the following warnings.

There are some potential concerns associated with the use of any sound generated by a tinnitus management device. Among them are the potential for worsening of tinnitus and/or a possible change in hearing thresholds.

Should you experience or notice a change in hearing or tinnitus, or any dizziness, nausea, headaches, heart palpitations or possible skin irritation at the point of contact with the device, you should immediately discontinue use of the device and seek a consultation with a medical, audiology, or other hearing care professional.

As with any device, misuse of the sound generator feature could present some potentially harmful effects. Care should be taken to prevent the unauthorized use and to keep the device out of the reach of children and pets.

Maximum wearing time

Always follow the maximum wearing time per day of the Tinnitus Sound-Support advised by your hearing care professional. Prolonged use may lead to worsening of your tinnitus or of your hearing loss.

You should familiarize yourself fully with the following general warnings before using your hearing aid for your personal safety and to ensure correct usage.

Please note that a hearing aid will not restore normal hearing and will not prevent or improve a hearing impairment resulting from organic conditions. Furthermore, note that in most cases, infrequent use of a hearing aid does not permit a user to attain its full henefits.

Consult your hearing care professional if you experience unexpected operations or events with your hearing aid.

Usage of hearing aids

Hearing aids should be used only as directed and adjusted by your hearing care professional. Misuse can result in sudden and permanent hearing loss.

Never allow others to wear your hearing aid as incorrect usage could cause permanent damage to their hearing.

Choking hazards & risk of swallowing batteries and other small parts

Hearing aids, their parts, and batteries should be kept out of reach of children and anyone who might swallow these items or otherwise cause injury to themselves.

Batteries have occasionally been mistaken for pills. Therefore, check your medicine carefully before swallowing any pills.

Most hearing aids can be supplied with a tamper-resistant battery drawer upon request. This is strongly recommended for infants, small children, and people with cognitive impairments.

Children younger than 36 months must

always use a tamper-resistant battery drawer. Please talk to your hearing care professional about the availability of this option.

If a battery or hearing aid is swallowed, see a doctor immediately and contact the National Poison Center at 1-800-222-1222 or National Battery Ingestion Hotline at 202-625-3333.

Battery use

Always use batteries recommended by your hearing care professional. Low quality batteries may leak and cause bodily harm.

Never attempt to recharge your batteries, and never dispose of batteries by burning them. There is a risk that the batteries will explode.

Dysfunction

Be aware of the possibility that your hearing aid may stop working without

notice. Keep this in mind when you depend on warning sounds (e.g. when you are in traffic). The hearing aids may stop functioning, for instance if the batteries have expired or if the tubing is blocked by moisture or earwax.

Active implants

The hearing aid has been thoroughly tested and characterized for human health according to international standards for human exposure (Specific Absorption Ratio - SAR), induced electromagnetic power and voltages into the human body.

The exposure values are well below international accepted safety limits for SAR, induced electromagnetic power and voltages into the human body defined in the standards for human health and coexistence with active medical implants, such as pacemakers and heart defibrillators.

If you have an active brain implant, please contact the manufacturer of your implantable device for information about the risk of disturbance.

The Auto Phone magnet and MultiTool (which has a built-in magnet) should be kept at least 12 in. away from the implant, e.g. do not carry it in a breast pocket.

X-ray, CT, MR, PET scanning, and electrotherapy

Remove your hearing aid before X-ray, CT/MR/PET scanning, electrotherapy, surgery, etc. as your hearing aid may be damaged when exposed to strong electromagnetic fields.

Heat and chemicals

The hearing aid must never be exposed to extreme heat, e.g. left inside a parked car in the sun.

The hearing aid must not be dried in microwave ovens or other ovens.

The chemicals in cosmetics, hairspray, perfume, aftershave lotion, sunscreen lotion, and insect repellent can damage the hearing aid. Always remove your hearing aid before applying such products and allow time to dry before use.

Power instrument

Special care should be exercised when selecting, fitting and using a hearing aid when the maximum sound pressure capability exceeds 132 dB SPL (IEC 711), as there may be risk of impairing the remaining hearing of the hearing aid user.

For information of whether your hearing aid is a power instrument, see the model overview in the front of this booklet.

Possible side effects

Hearing aids and earpieces may cause an accelerated accumulation of earwax.

The otherwise non-allergenic materials used in hearing aids may in rare cases cause skin irritation or other side effects.

Please consult a physician if these conditions occur.

Interference

The hearing aid has been thoroughly tested for interference, in accordance with the most stringent international standards. However, interference between the hearing aid and other devices (e.g. some mobile telephones, citizens band systems, shop alarm systems and other devices) may occur. If this occurs, increase the distance between the hearing aid and the interfering device.

Use on aircraft

Your hearing aid has Bluetooth. On board an aircraft, flight mode must be activated, unless Bluetooth is permitted by the flight personnel.

Connection to external equipment

The safety of the hearing aid when connected to external equipment with an auxiliary input cable, is determined by the external signal source. When connected to external equipment plugged into a wall outlet, this equipment must comply with IEC-62368 (or IEC-60065, IEC-60950 until June 20, 2019) or equivalent safety standards.

Warnings to hearing care professional

A hearing care professional should advise a prospective hearing aid user to consult immediately with a licensed physician (preferably an ear specialist) before dispensing a hearing aid if the hearing care professional determines through inquiry, actual observation, or review of any other available information concerning the prospective user, that the prospective user has any of the following conditions:

- (i) Visible congenital or traumatic deformity of the ear.
- ii) History of active drainage from the ear within the previous 90 days.

- (iii) History of sudden or rapidly progressive hearing loss within the previous 90 days.
- (iv) Acute or chronic dizziness.
- (v) Unilateral hearing loss of sudden or recent onset within the previous 90 days.
- vi) Audiometric air-bone gap equal to or greater than 15 decibels at 500 Hertz (Hz), 1,000 Hz, and 2,000 Hz.
- (vii) Visible evidence of significant cerumen accumulation or a foreign body in the ear canal.
- (viii) Pain or discomfort in the ear.

Special care should be exercised in selecting and fitting a hearing aid whose maximum sound pressure capability exceeds 132 dB SPL as there may be risk of impairing the remaining hearing of the hearing aid user.

Important notice for prospective hearing aid users

Good health practice requires that a person with a hearing loss have a medical evaluation by a licensed physician (preferably a physician who specializes in diseases of the ear) before purchasing a hearing aid. Licensed physicians who specialize in diseases of the ear are often referred to as Otolaryngologists, Otologists or

Otorhinolaryngologists. The purpose of medical evaluation is to ensure that all medically treatable conditions that may affect hearing are identified and treated before the hearing aid is purchased. Following the medical evaluation, the physician will give you a written statement that states that your hearing loss has been medically evaluated and that you may be considered a candidate for a hearing aid. The physician will refer you to an audiologist or a hearing aid dispenser, as appropriate, for a hearing aid evaluation.

The audiologist or hearing care professional will conduct a hearing aid evaluation to assess your ability to hear with and without a hearing aid. The hearing aid evaluation will enable the audiologist or dispenser to select and fit a hearing aid to your individual needs. If you have reservations about your ability to adapt to amplification, vou should inquire about the availability of a trial, rental or purchaseoption program. Many hearing care professionals now offer programs that permit you to wear a hearing aid for a period of time for a nominal fee, after which you may decide if you want to purchase the hearing aid. Federal law limits the sale of hearing aids to those individuals who have obtained

a medical evaluation from a licensed physician.

Federal law permits a fully informed adult to sign a waiver statement declining the medical evaluation for religious or personal beliefs that preclude consultation with a physician. The exercise of such a waiver is not in your best health interest and its use is strongly discouraged. A hearing aid will not restore normal hearing and will not prevent or improve a hearing impairment resulting from organic conditions. A hearing aid is only part of hearing rehabilitation and may need to be supplemented by auditory training and lip reading.

Children with hearing loss

In addition to seeing a physician for medical evaluation, a child with a hearing loss should be directed to an audiologist for evaluation and rehabilitation, since hearing loss may cause problems in language development and educational and social growth of a child. An audiologist is qualified by training and experience to assist in the evaluation and rehabilitation of a child with a hearing loss. If the user is an infant, small child, or person with cognitive impairment, it is recommended that the hearing aid be modified with a tamper-resistant battery compartment.

Troubleshooting

Symptom	Possible causes	Solutions
No sound	Dead battery	Replace the battery
	Clogged earpieces (dome, Grip Tip, earmold or MicroMold)	Clean earmold or MicroMold or replace wax filter
	clogged earpieces (dollie, drip 11p, earlifold of MicroMold)	Consider to replace dome, or GripTip
	Hearing aid microphone muted	Unmute the hearing aid microphone
Intermittent or	Clogged sound outlet	Clean earmold or MicroMold, replace wax filter or change dome or GripTip
reduced sound	Moisture	Wipe battery with a dry cloth
Squealing noise	Hearing aid earpiece inserted incorrectly	Re-insert the earpiece
	Earwax accumulated in ear canal	Have ear canal examined by your doctor
	Ear has grown	Contact your hearing care professional
Beeping/LED blinking (optional)		
Pairing issue with Apple device	Bluetooth connection failed	1) Unpair your hearing aid (Settings→General→Accessibility→Hearing Devices→Devices
	Only one hearing aid paired	→Forget this device). 2) Turn Bluetooth off and on again. 3) Open and close battery drawer on hearing aid. 4) Re-pair hearing aid (see chapter: "Pair with iPhone")
		If none of the above colutions work consult your bearing care professional

Water and dust resistant (IP68)

Your hearing aid is dust tight and protected against ingress of water, which means it is designed to be worn in all daily life situations. Therefore, you do not have to worry about sweat or getting wet in the rain. Should your hearing aid come into contact with water and stop working, please follow these quidelines:

- 1. Gently wipe off any water.
- 2. Open the battery drawer, remove the battery, and gently wipe off any water in the battery drawer.
- 3. Let the hearing aid dry with the battery drawer left open for approximately 30 minutes.
- 4. Insert a new battery.

IMPORTANT NOTICE

Do not wear your hearing aid while showering or participating in water activities. Do not immerse your hearing aid in water or other liquids.

Conditions of use

Operating conditions	Temperature: +34°F to +104°F Relative humidity: 5% to 93%, non-condensing
Storage and transport conditions	Temperature and humidity shall not exceed the below limits for extended periods during transport and storage:
	Temperature: -13°F to +140°F Relative humidity: 5% to 93%, non-condensing

Warranty

Certificate

Name of owner:		
Hearing care professional:		
Hearing care professional's address:		
Hearing care professional's phone:		
Purchase date:		
Warranty period:	Month:	
Model left:	Serial no.:	
Model right:	Serial no.:	

International warranty

Your hearing aid is covered by an international limited warranty issued by the manufacturer for a period of at least 12 months from the date of delivery. This limited warranty covers manufacturing and material defects in the hearing aid itself, but not in accessories such as batteries, tubing, speakers, earpieces and filters, etc. Problems resulting from improper or incorrect handling or care, excessive use, accidents, repairs made by an unauthorized party, exposure to corrosive conditions, physical changes in your ear, damage due to foreign objects entering the device, or incorrect adjustments are NOT covered by the limited warranty and may void it. The above warranty does not affect

any legal rights that you might have under applicable national legislation governing sale of consumer goods. Your hearing care professional may have issued a warranty that goes beyond the clauses of this limited warranty. Please consult him/her for further information.

If you need service

Take your hearing aid to your hearing care professional, who may be able to sort out minor problems and adjustments immediately.

Mobile phone

Some hearing aid users have reported a buzzing sound in their hearing aid when they are using mobile phones, indicating that the mobile phone and hearing aid may not be compatible.

The ANSI C63.19 standard determines the prediction of compatibility between a specific hearing aid and a mobile phone by: adding the numerical value of the rating for the hearing aid immunity to the numerical value of the rating for the mobile phone emissions. A sum of 4 would indicate that the combination of wireless device and hearing aid is usable; a combined rating that equals at least 5 would provide normal use; a combined rating of 6 or greater would indicate excellent performance.

Whereas all hearing aids have acoustic coupling, only the larger hearing aids have the physical space for telecoil (inductive) coupling. These two types of coupling have different rating scales (M1-M4 for acoustic coupling and T1-T4 for telecoil coupling, respectively) and both ratings are therefore relevant when predicting the compatibility of a particular hearing aid.

For a hearing aid with both acoustic coupling and telecoil coupling with a rating of M4/T2 and with a telephone rating of M3/T3), the combined rating is 7 (M4 + M3) for the acoustic coupling and 5 (T2 + T3) for the telecoil coupling. According to the guidelines given above, both types of coupling

will thereby be acceptable, with the acoustic coupling indicating excellent performance and the telecoil coupling indicating normal use.

The above equipment performance measurements, categories and system classifications are based upon the best information available, but it cannot be guaranteed that all users will be satisfied.

The immunity of this hearing aid is at least M2/T2.

The equipment performance measurements, categories and system classifications are based upon the best information available but cannot guarantee that all users will be satisfied.

IMPORTANT NOTICE

The performance of individual hearing aids may vary with individual mobile phones. Therefore, please try this hearing aid with your mobile phone or, if you are purchasing a new phone, be sure to try it with your hearing aid prior to purchase. For additional guidance, please ask your mobile phone provider for the booklet entitled "Hearing Aid Compatibility with Digital Wireless Cell Phones."

Technical information

The hearing aid contains two radio technologies, which are described below:

The hearing aid contains a radio transceiver using short-range magnetic induction technology working at 3.84 MHz. The magnetic field strength of the transmitter is very weak and is always below 15 nW [typically below -40 dBµA/m at a 10 meter/33 ft. distance].

The hearing aid also contains a radio transceiver using Bluetooth Low Energy (BLE) and a proprietary short-range radio technology both working at ISM band 2.4 GHz. The radio transmitter is weak and always

below 3 mW equal to 4.8 dBm in total radiated power.

The hearing aid complies with international standards concerning electromagnetic compatibility and human exposure.

Due to the limited space available on the hearing aid, relevant approval markings can be found in this document.

Additional information can be found in the "Technical Data sheet" on www.oticon.com

USA and Canada

The hearing aid contains a radio module with the following certification ID numbers:

FCC ID: U28AUBTEP IC: 1350B-AUBTEP

The device complies with Part 15 of the FCC Rules and with Industry Canada's license-exempt RSSs. Operation is subject to the following two conditions:

- 1. This device may not cause harmful interference.
- This device must accept any interference received, including interference that may cause undesired operation.

Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

This Class B digital apparatus complies with Canadian ICES-003.

Note: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions. may cause harmful interference to radio communications. However, there is no quarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined

by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the manufacturer or an experienced radio/TV technician for help.

The manufacturer declares that this hearing aid is in compliance with the essential requirements and other relevant provisions of Directive 2014/53/EU.

Declaration of Conformity is available from the manufacturer.



Manufactured by: Oticon A/S Kongebakken 9 DK-2765 Smørum Denmark www.oticon.global

CE 0543



Waste from electronic equipment must be handled according to local regulations.







Description of symbols used in this booklet



Warnings

Manufacturer

Text marked with a warning symbol must be read before using the device.



The device is produced by the manufacturer whose name and address are stated next to the symbol. Indicates the medical device manufacturer, as defined in EU Directives 90/385/EEC, 93/42/EEC and 98/79/EC.

CE mark



C € 0543 The device complies with Medical Device Directive 93/42/EEC. The four digit number indicates the identification of the notified body.



Electronic waste (WEEE)

Recycle hearing aids, accessories or batteries according to local regulations. Hearing aid users can also return electronic waste to their hearing care professional for disposal. Electronic equipment covered by Directive 2012/19/EU on waste and electrical equipment (WEEE).



Regulatory Compliance Mark (RCM)

The device complies with electrical safety, EMC and radio spectrum requirements for devices supplied to the Australian or New Zealand market.

IP code



Indicates the class of protections against harmful ingress of water and particulate matter according to EN 60529:1991/A1:2002.

IP6X indicates total dust protection. IPX8 indicates the protection against the effects of continuous immersion in water.

Bluetooth logo



Bluetooth* Registered trademark of Bluetooth SIG, Inc. where any use of such requires a license



Made for Apple badges

Indicates that the device is compatible with iPhone, iPad and iPod touch.

Description of symbols used on the regulatory packaging label



Keep dry

Indicates a medical device that needs to be protected from moisture.



Caution symbol

Consult instructions for use for warnings and cautions.



Catalog number

Indicates the manufacturer's catalog number so that the medical device can be identified.



Serial number

Indicates the manufacturer's serial number so that a specific medical device can be identified.

Your individual hearing aid settings

To be filled out by your hearing care professional.

Tinnitus SoundSupport: Limitation on use			
No limitation on use			
Program	Start-up volume (Tinnitus) Max volume (Tinnitus)		
1	Max hours per day	Max hours per day	
2	Max hours per day	Max hours per day	
3	Max hours per day	Max hours per day	
4	Max hours per day	Max hours per day	


Settings overview for your hearing aid				
Left Right				
☐ Yes	□No	Volume control	☐ Yes	□No
☐ Yes	□No	Program shift	☐ Yes	□No
☐ Yes	□No	Mute	☐ Yes	□No
☐ Yes	□No	Tinnitus SoundSupport	☐ Yes	□No
Volume control indicators				
□On	☐ Off	Beeps at min/max volume	☐ On	☐ Off
□On	☐ Off	Beeps when changing volume	□ On	☐ Off
□On	☐ Off	Beeps at preferred volume	☐ On	☐ Off
Battery indicators				
□On	☐ Off	Low battery warning	□ On	☐ Off

Technical Data

BTE13 PP

105

2CC Coupler measured according to American National Standard ANSI S3.22-2014 and ANSI S3.55-2014/Part 5. Supply voltage: Battery Zinc Air 1.4 Volt

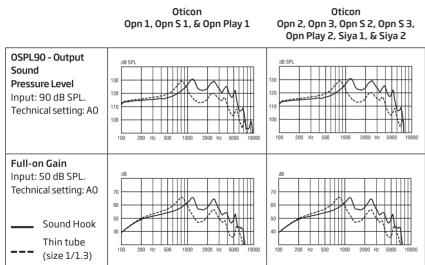




0 dB SPL ref. 20 mPa	Oticon Opn 1, Opn S 1, & Opn Play 1	Oticon Opn 2, Opn S 2 & Siya 1	Oticon Opn 3, Opn S 3, Opn Play 2, & Siya 2
Peak OSPL90	131 (1291) dB SPL	131 (129*) dB SPL	131 (129*) dB SPL
HF Average OSPL90	126 (118¹) dB SPL	126 (118*) dB SPL	126 (118*) dB SPL
Peak Full-on Gain	66 (66¹) dB	66 (66*) dB	66 (66*) dB
HF Average Full-on Gain	61 (54 ¹⁾ dB	61 (54*) dB	61 (54*) dB
Reference Test Gain	50 dB	50 dB	50 dB
Frequency Range	120-7000 Hz	120-7000 Hz	120-7000 Hz
Total Harmonic Distortion 500 Hz	3 %	3 %	3%
Total Harmonic Distortion 800 Hz	<2%	<2%	<2%
Total Harmonic Distortion 1600 Hz	<2%	<2%	<2%
Battery Consumption	1.9 mA	1.9 mA	1.9 mA
Equivalent Input Noise Level (omni/dir)	14/27 dB SPL	14/27 dB SPL	14/27 dB SPL
HF Average SPLITS (left/right ear)	109/109 dB SPL	109/109 dB SPL	109/109 dB SPL
Attack Time	<5 ms	<5 ms	<5 ms
Release Time	<50 ms	<50 ms	< 50 ms

^{*} For instruments fitted with thin tube

2CC Coupler measured according to American National Standard ANSI S3.22-2014 and ANSI S3.55-2014/Part 5. Supply voltage: Battery Zinc Air 1.4 Volt

Siya 1 & 2 **2CC Coupler**



dB SPL ref. 20 mPa	Oticon Siya 1 & Siya 2

Peak OSPL90	120 (121*) dB SPL
HF Average OSPL90	115 (105*) dB SPL
Peak Full-on Gain	57 (54*) dB
HF Average Full-on Gain	50 (41*) dB
Reference Test Gain	39 dB
Frequency Range	100-7000 Hz
Total Harmonic Distortion 500 Hz	<2%
Total Harmonic Distortion 800 Hz	<2%
Total Harmonic Distortion 1600 Hz	<2%
Battery Consumption	1.7 mA
Equivalent Input Noise Level (omni/dir)	18/28 dB SPL
HF Average SPLITS (left/right ear)	97/97 dB SPL
Attack Time	<5 ms
Release Time	<30 ms
Kelease I lille	לווו חרי

^{*} For instruments fitted with thin tube



