B71 Bone Transducers

#8506731 (10 ohm), #8506732 (50 ohm), #8506735 (150 ohm), #8506736 (300 ohm)

Features

- Reliable performance
- RoHS compatible
- Outstanding quality
- Biocompatible case
- ANSI and ISO compliant
- IEC 60601-1-2 4th edition compliant
- IEC60601-1 safety compliant



The Gold

Standard

of Audiometric Transducers

RadioEar Bone Transducers


Since its introduction in the 1970s the RadioEar B71 has been the bone transducer of choice for audiometric testing. As a consequence of ever changing standards we continuously endeavour to update our product, so that it is compliant with all the latest regulations. RadioEar has an extensive history of successfully serving the audiometric industry. We recognize the critical importance these devices have for our customers, and are sincerely dedicated to serving them.

- Unsurpassed in consistent reliable performance
- Fabricated and hand assembled in the US
- Available in custom impedances up to 300 ohm
- Subject to change



Technical Specifications

Typical Response Curve

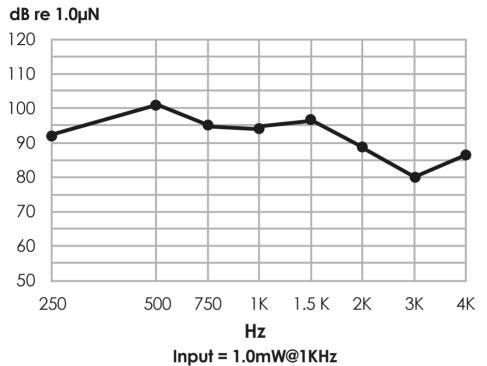

Standards


- ISO 389-3:1994(E) ANSI \$3.6-2010, IEC 60645-1:2012 and IEC 60645-2:1993
- Common impedances: 10, 32, 50, 100, 300 ohms @ 1 kHz (custom impedances available)
- Frequency response: 250-4000 Hz
- Max Input Voltage: 20 dB re 1.0 mW
- Biocompatibility: no biological effects as per ISO 10993-1:2009
- Weight: 24 g (0.846 oz)
- Connector: 2 pin plug with safety fixation point

Harmonic Distortion

Frequency Hz	250	500 & 750	1K - 4K
Hearing Level	20	50	50
T.H.D.% Typical	2.3	<1.1	<0.3
T.H.D.% Maximum	5.5	5.5	5.5

All measurements performed on Brüel & Kjær Type 4930 Artificial Mastoid with 5.4N static load.

Test results for individual, serialized, bone transducers are available.



Physical dimensions of the bone transducer B71: H: 19mm W:19mm L: 32mm

Audiometric Calibration

Frequency Hz	mV	dB re 1.0mV
250	515.9	54.3
500	69.0	36.8
750	43.9	32.9
1000	25.5	28.1
1500	10.1	20.1
2000	11.8	21.4
3000	31.5	30.0
4000	27.2	28.7

The data above gives the required input voltage as measured at the bone transducer terminals to provide force levels 40dB nHL ± 3.0dB above threshold (RETFL) based on ISO and ANSI standards for a typical B71, 10 ohm impedance.

